

MICROTEK



ScanWizard *Bio*

Reference Manual

Copyright © 2014 by Microtek International, Inc.

All rights reserved.

Trademarks

Microtek, ScanMaker, ArtixScan, ScanWizard and ColoRescue are trademarks or registered trademarks of Microtek International, Inc. Adobe and Acrobat are registered trademarks of Adobe Systems Incorporated. Windows is a registered trademark of Microsoft Corporation. All other trademarks or registered trademarks are the property of their respective holders. Software function or specifications are subject to change without notice. Not responsible for typographical errors.

Important

Documents that you scan may be protected under copyright law. The unauthorized use of such documents could be a violation of the rights of the copyright holder. Microtek bears no responsibility for the unauthorized use of copyrighted materials.

To obtain optimal results from the Microtek scanning software and user's manual, you should be familiar with such Windows concepts as pointing, clicking, dragging, and selecting from menus and dialog boxes. If these things are new to you, refer to your Microsoft Windows User's Guide.

I49-004656 D

April 2014

Microtek International, Inc.

6, Industry East Road 3, Science Based Industrial Park, Hsinchu, 30077, Taiwan

Tel: 886-3-5772155, Fax: 886-3-5772598, <http://www.microtek.com>

Contents

Introduction	1
The ScanWizard Bio Interface	2
Launching the ScanWizard Bio	3
Exiting ScanWizard Bio	3
 The Preview Window	 4
Elements of the Preview Window	4
Preview Area	6
Scan Material	7
Unit of Measurement/Rulers	8
Overview, Prescan, and Scan to	9
Overview	9
Prescan	9
Scan to	9
Copy	10
E-mail	10
Toolbar	11
Scan Frame (Frame)	11
Zoom (Magnify Glass)	11
Move (Pan)	11
White/Black Points Pickers	12
Auto Focus	13
The Scanner Menu	15
Scanner Model	15
Get Current Scanner Info	15
Scanner Control (Power Saving Control)	16
Scanner Probe	16
The View Menu	17
Overview Image/Preview Image	17
Resize Window to Fit	18
Bring Settings Window to Front	18
Show/Hide Windows	18

The Preferences Menu	19
Scan Material	19
Calibration Setup	20
White/Black Points Setup	22
Cursor Auxiliary Lines	23
Overview Setup	24
Prescan Setup	26
Monitor Gamma Setup	27
Invert	27
More... command	28
The Correction Menu	31
The Help Menu	31
The Settings Window	32
Elements of the Settings Window	32
Scan Job	34
Image Type	35
Resolution Settings	36
Resolution List Box	36
Resolution Unit	37
Scan Frame and Related Settings	38
Scan Frame Settings	38
Scaling	38
Output Settings	39
Image Size	39
Unit of Measurement	39
Multiple Sampling	40
Channel	41
Custom	41
Transform	42
The Reset button	42
Advanced Image Correction Tools	43
Accessing the AIC Tools	44
Elements of AIC Dialog Box	45
The Action Buttons	47
Custom Settings	48
Adding Custom Settings	48

Removing Custom Settings	49
Loading/retrieving custom settings	49
White/Black Points	50
Tone Curve	53
Filter	57
Brightness and Contrast	59
Exposure Time (for Transmissive mode only)	60
Automatic Color Restoration	61
The Information Window	62
Elements of the Information Window	62
Zoom Level Display	63
Mouse Cursor Position	63
Color Output Meter	63
Sample Display Area	64
Color Meter Options	64
The Scan Job Queue Window	65
Elements of the Scan Job Queue window	65
One-pass Scan for Multiple Scan Jobs	67
Multiple Auto-crop for EZ-Lock Film Holder	68
Function Buttons	69
Selecting Multiple Scan Jobs	69
Editing Multiple Scan Jobs	69
Adding a New Scan Job	70
Duplicating a Scan Job	70
Removing a Scan Job	70
Checking a Scan Job	71
The Up/Down Arrows	71
The Load/Save Button	72
Appendix	
Product and Technical Support	74

Introduction

The ScanWizard Bio is a scanning software which is specifically designed for the use of the electrophoresis gel scanning. This manual covers the various commands and features found in the ScanWizard Bio scanning software for the Windows system. The manual information is divided into four major sections, corresponding to the four major windows of the program:

- Preview
- Settings
- Information
- Scan Job Queue




The ScanWizard Bio Interface

ScanWizard Bio consists of four major windows: Preview, Settings, Information, and Scan Job Queue.


All four windows appear automatically after ScanWizard Bio is started up the first time. You may hide or show the Scan Job Queue and Information windows by clicking on the *Hide/Show* toggle commands in the View menu of the Preview window.

Settings window contains scanning parameters for outputting the image and includes image correction tools


Scan Job window provides key functions in managing scan jobs

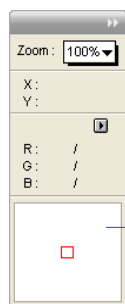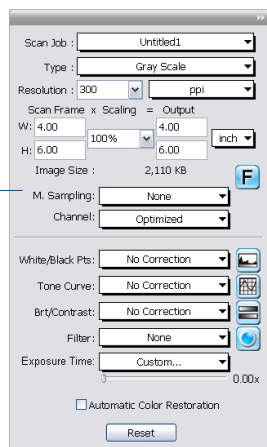

Information window provides information on the Preview image

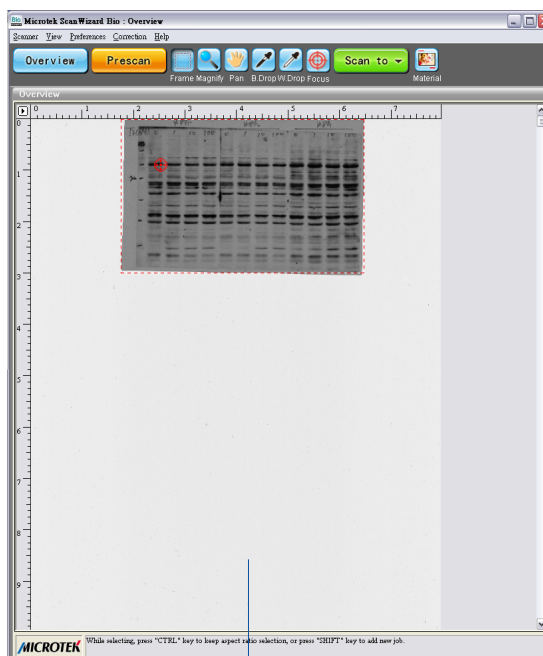

Preview window has commands and tools for controlling the scanner



Launching ScanWizard Bio

ScanWizard Bio can be launched in either Stand-alone or Plug-in mode.

- From Stand-alone mode: Double-click the *ScanWizard Bio* icon on the desktop, or choose *Start, Programs, Microtek ScanWizard Bio for Windows*, and then *ScanWizard Bio*
- From Plug-in mode: Choose the *Import* or *Acquire* command from the File menu of your image-editing software, then select *Microtek ScanWizard Bio*.

Exiting ScanWizard Bio


To exit ScanWizard Bio, double click on the *Close* box on the upper left side of the Preview window.



Click here to exit
ScanWizard Bio

The Preview Window

The Preview window is the most prominent window of the four major windows, and it includes the various commands and tools for controlling the scanner.

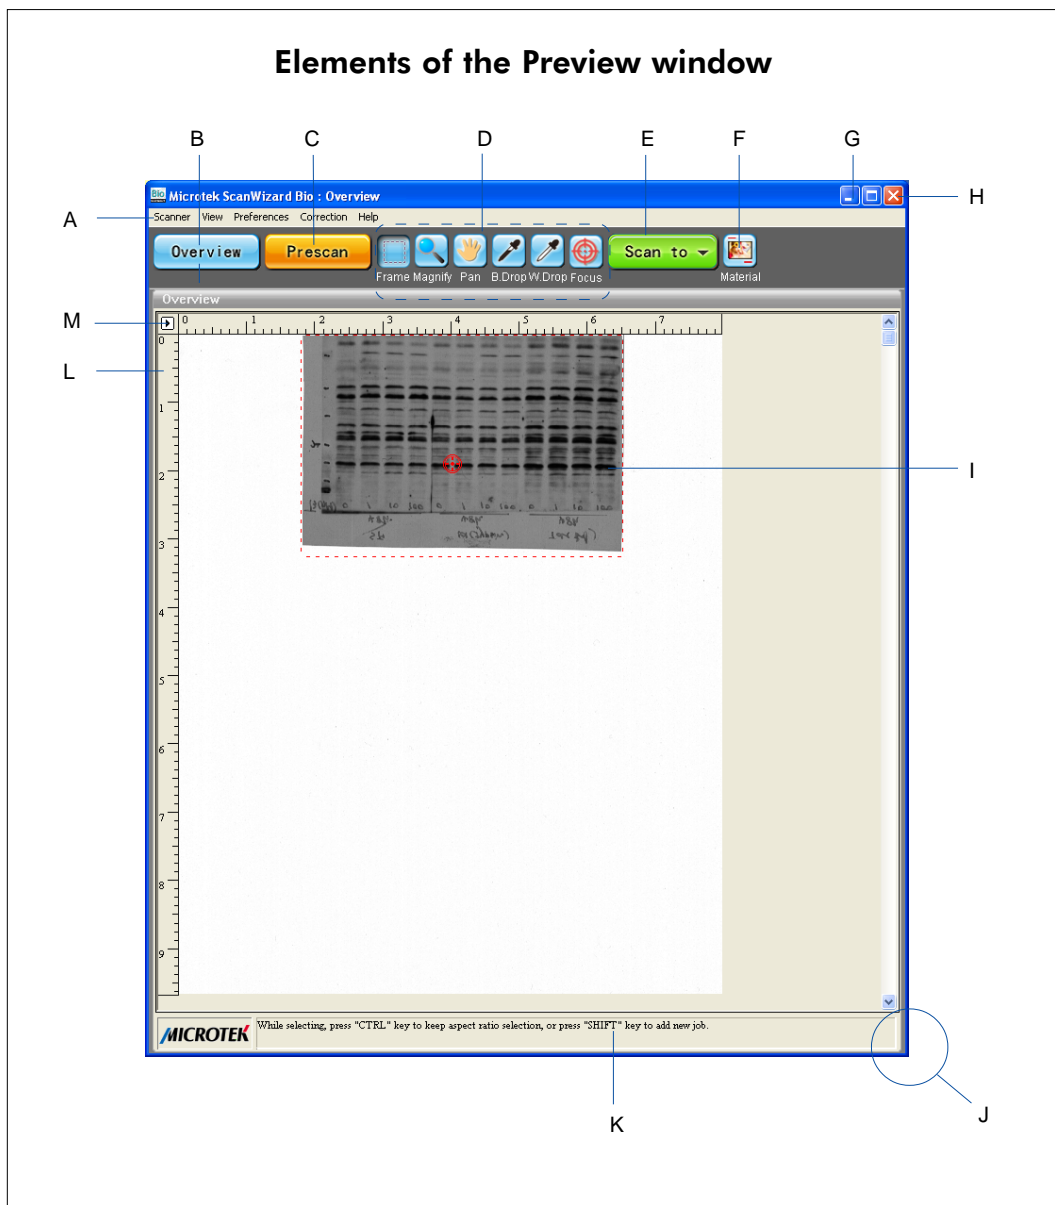


- A. Menu bar: The Menu bar includes the different menus for setting up the scanner (Scanner menu), controlling view options (View menu), customizing the software (Preferences menu), Image Correction function (Correction menu), and accessing on-line help (Help menu).
- B. Overview button: This button previews the specified or entire scan bed.
- C. Prescan button: This button previews one or more detailed images of the area(s) selected by the Frame (Scan Frame) tool.
- D. Toolbar: The buttons in the Toolbar perform specific actions on the overview image. Tool buttons include the Scan Frame (Frame) tool, Zoom (Magnify Glass) tool, Move (Pan) tool, Pickers tool and Auto Focus (AF) tool.
- E. Scan to button: This button starts the final scanning process.
- F. Scan Material button: This shows the type of your scan material – Reflective (photos and prints) or Transmissive (electrophoresis gels and slides).
- G. Minimize button: Click it to minimize ScanWizard Bio.
- H. Exit button: Click it to close ScanWizard Bio. Take note that when you exit, you quit from ScanWizard Bio scanning software.
- I. Preview area: The overview image is displayed in this area after you perform a scan.
- J. Resize: To increase or decrease the preview window, drag the bottom right corner of the window to resize.
- K. Status bar: This area shows you information pertinent to the operation underway or being performed.
- L. Rulers: Rulers are located on both sides of the Preview window to help you with measurement and alignment.
- M. Unit of Measurement: Select the unit of measurement for the rulers by clicking the arrow button at the 0,0 point of the rulers and choosing from the drop-down menu.

Preview Area

The preview area is where the overview or prescan image appears after you click either Overview, Prescan, or Scan to button.

By the default, the maximum size of the preview area is determined by your scanner's bed size (or maximum scan area) . For example, if the scanner's maximum scan area is 14" x 17", the maximum size of the preview area will be limited under this dimension.

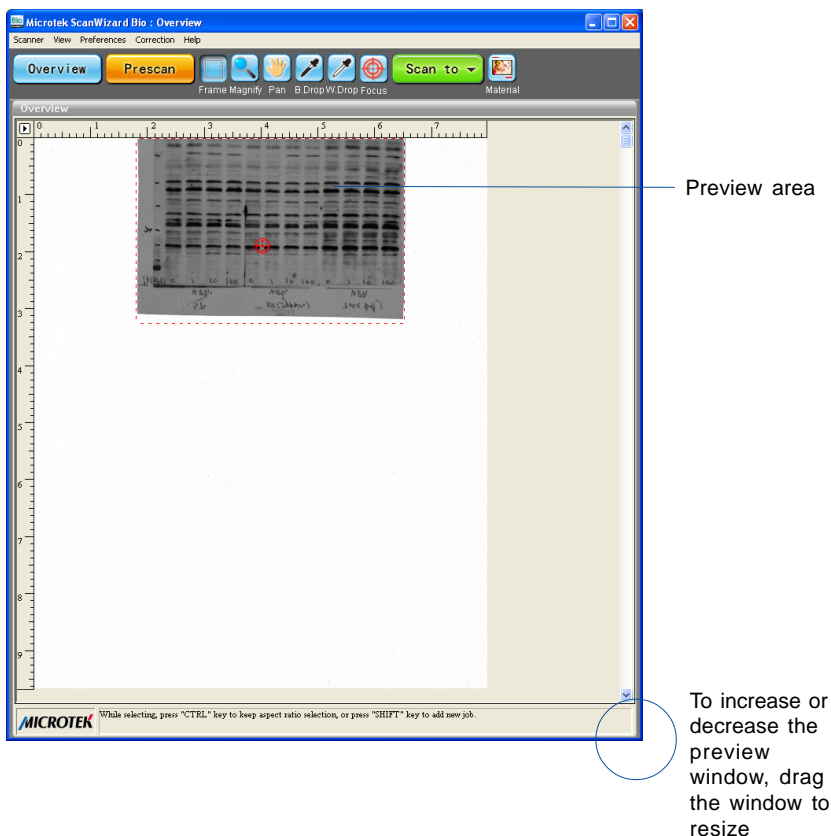

Scan Material

The Scan Material icon accesses the Scan Material menu. The appearance of the Scan Material icon changes, depending on whether the scan material is reflective or transmissive film.



If you are scanning reflectives (such as photos or printed materials), this is the appearance of the Scan Material icon. When you click the icon and hold down the mouse, you will see the Reflective option checked.



If you are scanning positive films (such as electrophoresis gels or slides), this is the appearance of the Scan Material icon. When you click the icon and hold down the mouse, you will see the Transmissive option checked.

Unit of Measurement/Rulers


The rulers on both sides of the preview window assist you in measurement or in checking the alignment of your image.

The unit of measurement in the ruler can be selected in two ways: in the Image Dimension controls located in the Settings window, or by clicking the ruler unit button at the 0,0 point of the rulers in the Preview window.

Depending on your selection, the rulers can mark off measurement in these units: inch, centimeter, millimeter, point, and pixel. The pixel option is dimmed if the selected resolution unit is lpi, and vice versa.

To select the unit of measurement for the rulers:

Click the unit box in the Settings window, or click the ruler unit button at the 0,0 point of the rulers in the Preview window. When the submenu appears, select the unit of measurement.

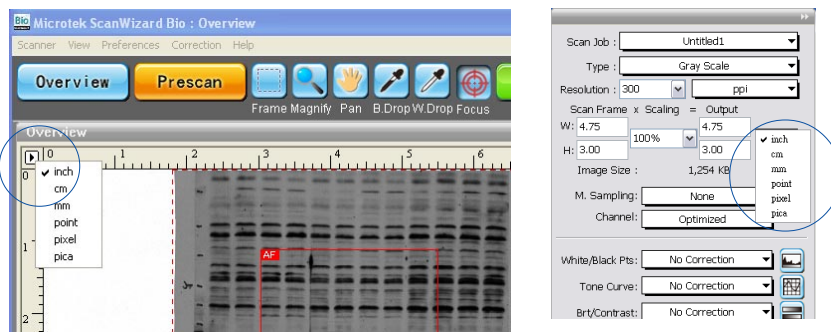

Overview, Prescan, Scan to

The Scan to button is one of ScanWizard Bio's great features, which functions the productivity tools under it. Click and hold the mouse button to activate Scan to options menu, you can select Scan to, Copy, or E-mail from the options provided.

Overview

Overview

The Overview button offers a preliminary and low-resolution overview of the image on the scan bed. By the default, the entire scan bed is previewed when you click the Overview button. You are not allowed to change the area size to be previewed in the Preview window.

Prescan

Prescan


The Prescan button offers a high-resolution preview image of the area selected by the scan frame tool. Multiple prescans can be done if you have several selected scan jobs. The prescans are performed one by one in an order that they are listed in the Scan Job Queue window.

Scan to

Scan to

This is the default button when ScanWizard Bio is launched as a stand-alone program (e.g., launched from the Start menu or the ScanWizard Bio icon on the desktop) when scanning reflective materials. It performs the final scan and delivers the scanned images to your selected folder or application.

When the “Scan To: Save As” dialog box appears, key in a file name, then select .tif, .bmp, .pcx, .dcx, .pdf, or other as the export file format, and click Save to perform the final scan.

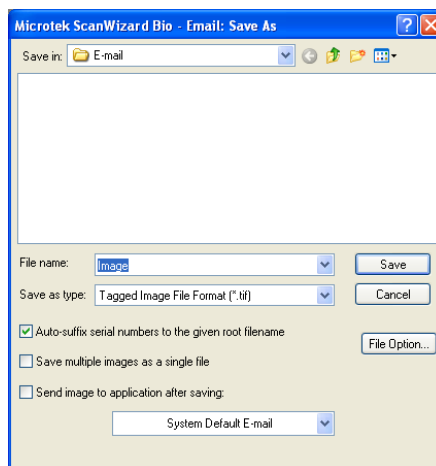




Copy

Click the Scan To button and hold down the mouse until the options menu appears, then select Copy. A scan is then performed, and the scanned image is sent to the specified printer.

When the “Copy” dialog box appears, select a default printer from the options. Specify the number of copies to be made, then click OK.

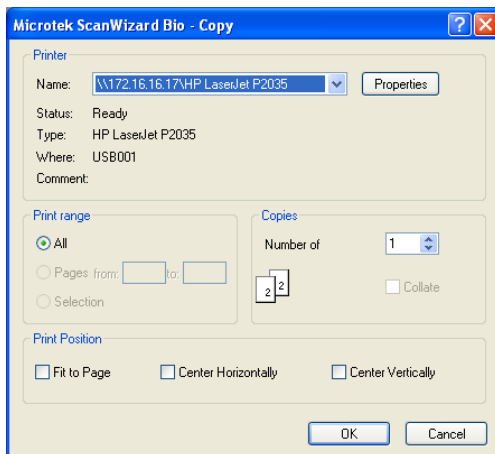


E-mail

Click the Scan To button and hold down the mouse until the Options menu appears, then select E-mail.


When the “E-mail: Save As” dialog box appears, key in a file name. It is recommended that you use either .jpg or .bmp as the file format.

Make sure that the check box “Send image to application after saving” has been checked. Then choose your preferred E-mail application from the options, and click Save. The saved file can now be attached to your E-mail message automatically.

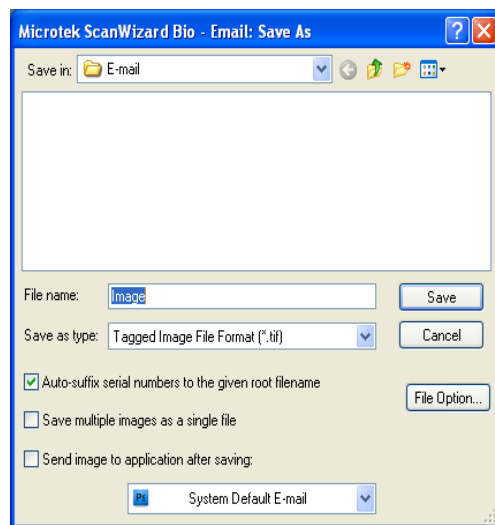

Toolbar

The Toolbar commands simplify the performance of certain tasks. The Toolbar commands include Scan Frame (Frame), Zoom (Magnify Glass), Move (Pan), Pickers and Auto Focus.

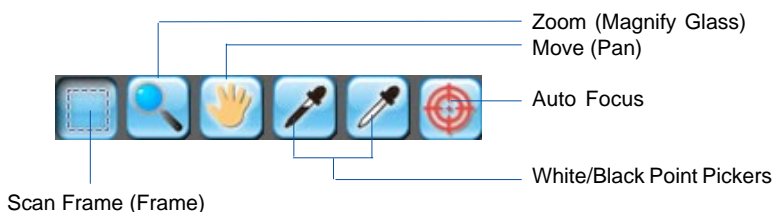

Scan Frame (Frame) tool

The Scan Frame tool lets you select the area to be scanned or prescanned. You can have multiple scan frames, but only one scan frame can be current at a time; the current scan frame is indicated by a flashing marquee. Multiple scan frames can be more easily distinguished if you turn on the *Smoked Glass Background* command (in the Preferences menu).

Zoom (Magnify Glass) tool

The Zoom tool lets you zoom in (magnify) and zoom out (reduce) your view of the image. Only your view of the preview image is changed; the actual size of the image remains unaffected. Each click of the zoom tool magnifies or reduces by a factor of 2. Thus, the magnification levels increase from 100% to 200%, to 400%, and to the maximum 800%. When you reach the maximum magnification factor, the center of the Zoom tool will appear empty.

To zoom out (reduce), hold down the Shift key and with the Zoom tool selected, click the image. A minus sign will be in the middle of the lens to indicate the image is being zoomed out.


Note: If the Info window is open, the zoom level will be indicated. This means you can also zoom in by selecting the appropriate zoom level in the Info window.


Move (Pan) tool

The Move tool lets you scroll through an overview or prescan image, allowing you to move parts of the image into view quickly without using the scroll bars. You can use the Move tool for scrolling through zoomed-in images that were enlarged through the Zoom tool, or for scrolling through parts of an image not included completely within the frame of the preview window.

White/Black Point Pickers

The Picker tools allow you to sample color from a particular area in an image, and are useful for designating shadow or highlight point.

The White Point Picker () lets you define the whitest reference point in the preview image. Once you have picked the whitest point, excessive white points are clipped off.

The Black Point Picker () lets you define the darkest reference point in the preview image. Once you have picked the darkest point, excessive black points are clipped off.

With the Picker tools, you can determine the color values for any pixel in an image. When you click the White/Black Picker and pan over a pixel, the value for that pixel is displayed in the Info window, based on the sample size selected in the Info window. Pixel value information is useful especially when you are making color adjustments based on color value.

To change the sample size of the Picker tool:

1. Open the Info window by choosing the Show Info Window command in the View menu.
2. Click the Color Meter Options button located to the right of the K values in the Info window.
3. Choose your options.

Select the sample size options from the drop-down list. For instance, the 1 by 1 option will display the value of one pixel — the pixel in the middle of the Color Output Meter. The 3 X 3 option reads the average value of a 3-pixel by 3-pixel area.

To display color information for a pixel or an averaged area:


1. Click the Picker tool.
2. As you pass over a point in the image, observe the Info window — the K values will be displayed in the Color Output Meter. These values are in turn based on the sample size you selected.

Auto Focus

The Auto Focus tool allows the scanner to change the focus position on images through the movement of the CCD, resulting in better image quality for a chosen area of the scan. You can either take the result which is the area applied with the Auto Focus function is decided and selected by the software system automatically, or assign a specific area of the scan frame applied with the Auto Focus function by yourself. This function tool is activated only for the scanners that support Auto Focus function (e.g., Bio-5000).

- The area applied with the Auto Focus function is decided and selected by the software system automatically.


Click the **Overview** button to perform a preliminary scan of the image, which will appear in the Preview window. Immediately, you can see a target sign (⊕) appearing on the overview image. The target sign marks the area where the Auto Focus is applied to. In this case, the software system automatically detects, calculates and selects the area applied with the Auto Focus function.

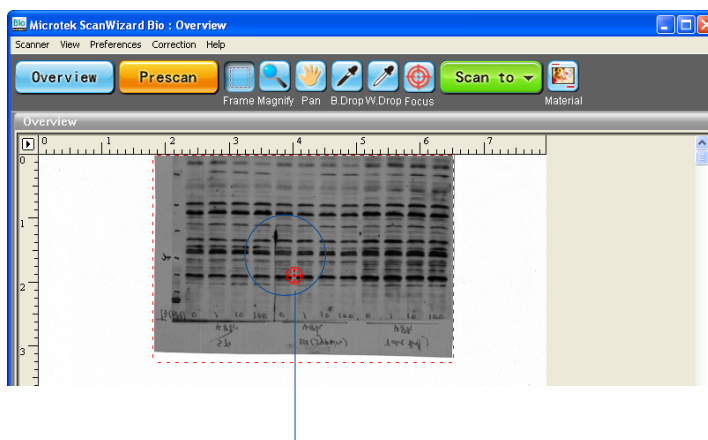

The target sign marks the area applied with the Auto Focus function, which is selected by the software system.


- Select and apply the Auto Focus function to a specific area of the scan frame by yourself.
 - a) Select the **Scan Frame** tool from the Toolbar in the Preview window, and choose the area to be scanned by dragging a rectangle around it.
 - b) Select the **Auto Focus** tool from the Toolbar in the Preview window, and select the area in the scan frame to which the AF function will be applied.

A redefined Auto Focus frame (bordered in red) will appear within the scan frame, labeled with the tag “AF”.

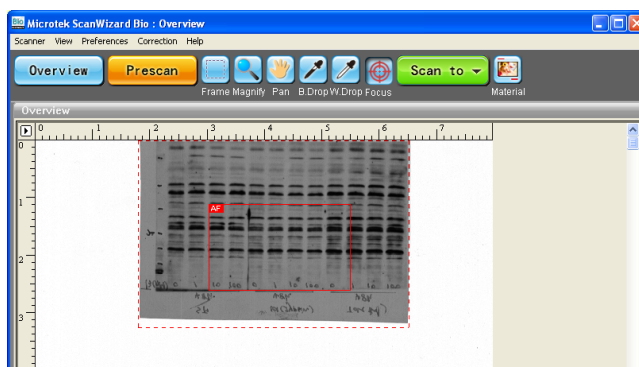


By the default, the Auto Focus function is not activated when your Scan Material is set as Reflective or Transmissive. If you like to apply the Auto Focus function to your scanned materials, you need to go to the Preference menu and to select the More command, and then check the Auto Focus to activate this option.


The Auto Focus function is not activated.

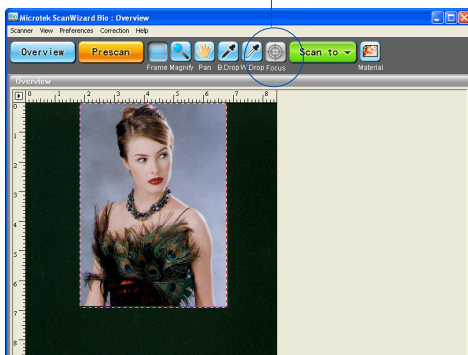

The Auto Focus function is activated.

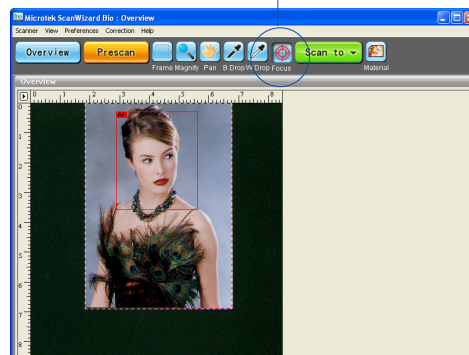

The Scanner Menu

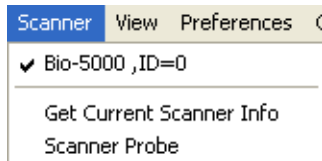

The Scanner Menu lets you:

- Show your scanner model or select a scanner if you have multiple scanners
- Get information about current scanner
- Get scanner information on the SCSI/USB/FireWire chain
- Set idle time for saving power


Scanner Model

The scanner model (and its SCSI, USB, or FireWire ID number) is shown at the top of the scanner. If you have multiple scanners on your system, all the scanners are shown with their respective IDs, and the current scanner is indicated by a check.

Only one scanner can be accessed at a time. To switch among various scanners, select the scanner to be used.

Get Current Scanner Info

This command provides information about your current scanner. When you choose this command, a dialog box appears showing the scanner model, Scanner ID number, and firmware version.

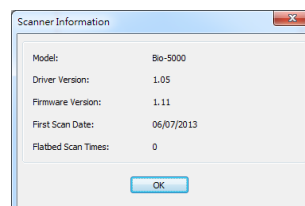


This information shows you how many scans have been passed through the roller, which helps out to accumulate the replacement point for the roller. The recommended replacement point is when the numbers on two sides of the slash symbol are equal. Press the Reset button to start recounting the scans for the roller after replacing a new one.

Scanner Control (Power Saving Control)


The power-saving feature of the scanner lamp to save energy and extend the life cycle of the lamp. By default, the lamp turns off automatically if the scanner is idle for 15 minutes. You can change the lamp idle time in your preferences or disable this feature completely by unchecking the *Auto Power Saving Mode* check box.

Note: Not all scanner models support these features. If your scanner model is not supported, the Scanner Controls command will be grayed out in the Scanner menu.

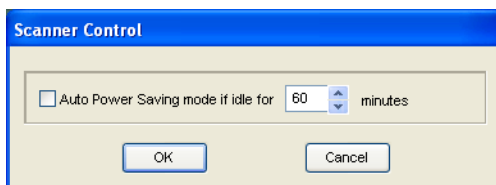


Scanner Probe

This command shows the scanner information on your SCSI, USB, or FireWire chain. If your scanner does not show in the Scanner List dialog box, make sure your scanner is properly installed, connected, and turned on, and then click the *Probe* button. For details on connecting your scanner, refer to your scanner hardware installation guide.

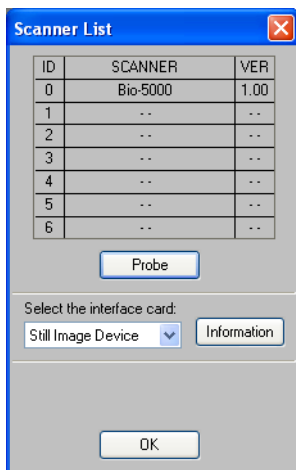

The View Menu

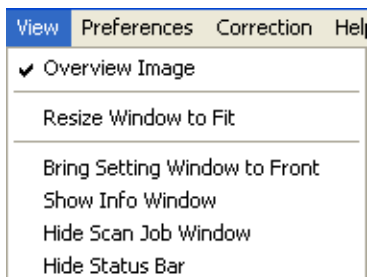

The View menu lets you:

- Resize the Preview window
- Show/hide the Information and Scan Job Queue window
- Show/hide Status Bar



Overview Image/Prescan Image

These commands allow you to switch between Overview or Prescan viewing modes.

- Overview image: This is an image obtained when you click the Overview button in the Preview window. The image shows you whatever is on your scan bed.


The Overview image is always checked automatically whenever you launch the ScanWizard Bio.

- Prescan image: This is a detailed image obtained from selecting an area in the Overview image and then clicking the Prescan button in the Preview window.

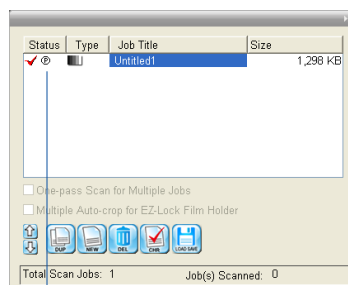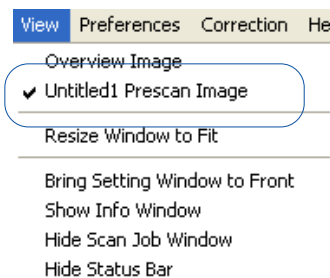


Click the Prescan button. The Prescan image will then be available for viewing in the View menu, and a "P" thumbnail will appear in the Scan Job Queue window.

Untitled1
Prescan Image

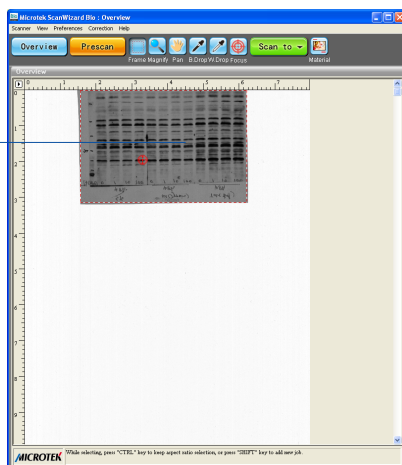

Overview viewing mode

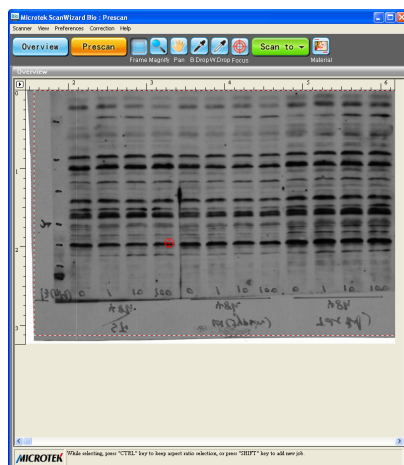

Prescan viewing mode

Resize Window to Fit

This command resizes the Preview window, which you may find helpful to do for conserving space on your desktop monitor (especially after you have enlarged the Preview window).

Bring Settings Window to Front

This command brings the Settings window to the forefront, which is useful if you have the Settings window hidden behind other windows or if you have expanded your Preview window such that it hides the Settings window in the background.

Show/Hide ...Window commands

These commands allow you to switch between showing or hiding the Scan Job Queue window, Information window, and Status bar on your screen.

To use this feature, choose the correct command from the View menu for viewing a window. When the window appears, you can hide it by choosing the particular Hide command for it.

The Preferences Menu



The Preferences menu lets you:

- Choose the correct scan material
- Set up White/black point parameters
- Reset calibration data
- Show/hide auxiliary cursor lines
- Fine-tune monitor gamma values
- Create the invert effect
- Activate the smoked glass effect
- Set other options, such as specifying a working directory for files

Scan Material

This command allows you to select the correct scan material. Scan materials can be classified into two types:


- Reflectives, such as medical reports, study reports, or prints.
- Positive films, such as electrophoresis gels or other X-ray films.

The default scan material is Positive Film no matter what scanner model you are using.

If you are scanning reflective materials, make sure that you switch to Reflective mode, or you will get inaccurate scanning results.

To choose your scan material:

- Choose the *Scan Material* command in the Preferences menu. From the submenu that appears, select your scan material; a check will appear next to the selected option.

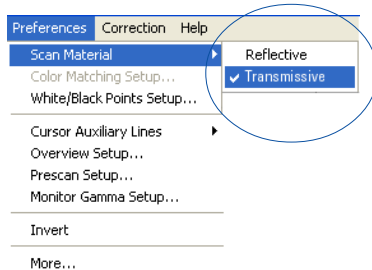


- Alternatively, you can click the *Scan Material* button and then choose the correct scan material from the drop-down menu that appears.



Calibration Setup

This command allows you to specify the calibration mode and reset the calibration data if needed.

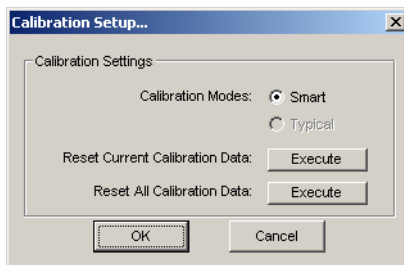

Calibration Modes

- **Smart:** If this mode is checked, when you use the ScanWizard Bio for the first time, you will be asked to calibrate your scanner and the system will generate and store a set of calibration data with different values of scan types and resolutions. Once the calibration data is made, you don't need to calibrate the scanner anymore even when the scan type and resolution are changed, enhancing scanning speed dramatically. This mode is always checked for some scanner models (e.g., Bio-6000, Bio-6000T).
- **Typical:** If this mode is checked, the ScanWizard Bio will need to re-calibrate your scanner and re-generate the calibration data every time when you start a new scanning job. This mode is always grayed out for some scanner models (e.g., Bio-6000, Bio-6000T)

Reset Current Calibration Data

This option allows you to remove the calibration data you are using presently; however, other calibration data you have created previously will not be affected. Once the current calibration data has been removed, you will need to calibrate the scanner again in order to retrieve the same calibration data.

To remove the current calibration data, click the “Execute” button next to the “Reset Current Calibration Data” option. The current calibration data file saved in “C:\Program Files\Microtek\ScanWizard Bio\Scanners” folder will be removed automatically.


Reset All Calibration Data

This option allows you to remove all calibration data from your system. Once all calibration data has been removed, you will need to re-calibrate the scanner and generate all new calibration data for your scanner once again.

To remove all calibration data, click the “Execute” button next to the “Reset All Calibration Data” option. The current calibration data file saved in “C:\Program Files\Microtek\ScanWizard Bio\Scanners” folder will be removed automatically.

White/Black Points Setup

This command provides you with advanced controls for setting the clipping points for your white and black points, as well as determining the output levels for the white/black points on your printer.

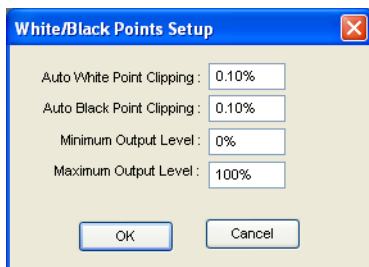

To use this feature:

1. Choose the *White/Black Points Setup* command from the Preferences menu.
2. As an alternative, you can click this command from the Color Correction Menu. This is also the same thing as clicking the White/Black points tool in the Settings window and then clicking the Setup button from the dialog box that comes up. When the dialog box comes up, specify your preferences.

Auto White Point Clipping/Auto Black Point Clipping

The *Auto White Point Clipping* and *Auto Black Point Clipping* fields allow you to specify the percentage by which the white and black points, respectively, can be clipped from the histogram. The clipping is done after you click the Auto button in the AIC White/Black Points dialog box.

For example, if you specify 10 percent as your White Point clipping value and then click the Auto button, the white point on the histogram is adjusted so that 10 percent of the color information is “clipped” or ignored. The resulting 90 percent information leftover is then remapped, resulting in an image with less highlight detail.

The same principle above applies to the Auto Black Point Clipping feature, which governs the black point for shadows.


Minimum Output Level/Maximum Output Level

The *Minimum Output Level* lets you set the minimum output level of the black point. The higher the percentage value, the lower the contrast will be.

The *Maximum Output Level* lets you set the output level of the white point. The lower the percentage value, the lower the contrast will be.

Cursor Auxiliary Lines

This command allows you to show or hide cursor auxiliary lines to help you define a scan frame or measurement off the rulers more precisely. Using the cursor auxiliary lines, you can also read the measurements of your ruler more easily.

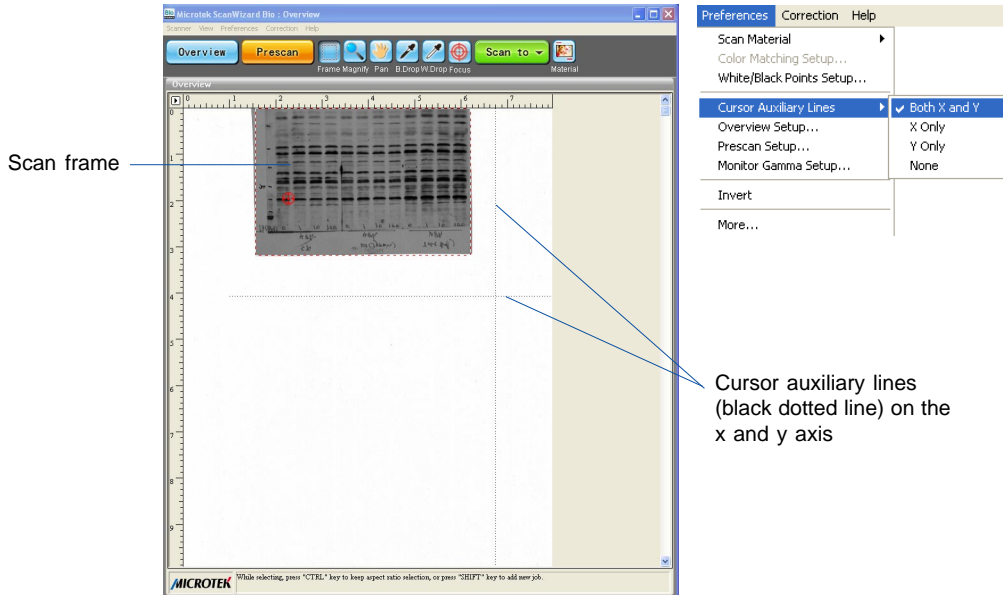


To use this feature:

1. Choose the Cursor Auxiliary Lines command in the Preferences menu.
From the submenu that appears, select how the cursor lines will appear.
 - On both x (horizontal) and y (vertical) axes
 - On x axis only
 - On y axis only
 - None (no cursor lines)
2. Click the Scan Frame tool.

To see how the cursor auxiliary lines work, draw a scan frame. Click on the top left corner of the image as your starting point, then drag down diagonally to form a scan frame. As you draw the scan frame, cursor lines will appear to help you draw the scan frame precisely. When you release the mouse, your scan frame will be aligned with the cursor lines.

Overview Setup


This command lets you set the area you want to be overviewed of the scan bed, and provides some overview options as well.

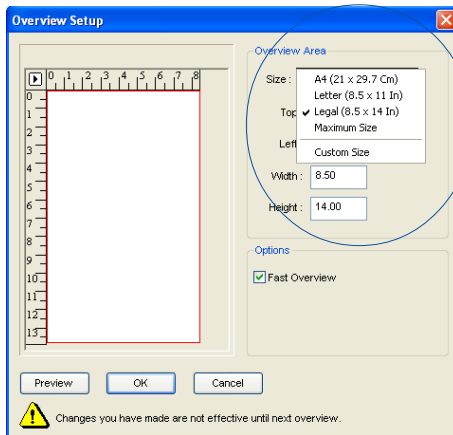

For scanning
reflectives

By default, ScanWizard Bio overviews the maximum scan area as determined by your scanner model's bed size. You can, however, customize the overview area so that the scanner consistently overviews only the specific dimensions you have in mind. For example, if your maximum scan area is 12" x 17", you can customize the overview area so that it consistently overviews, say, 8.5" x 11" of the bed size.

Note: If Transmissive is selected as your scan material, you can either select the Maximum size or define your preferred size by selecting the Custom from the Size option menu in the Overview Area .

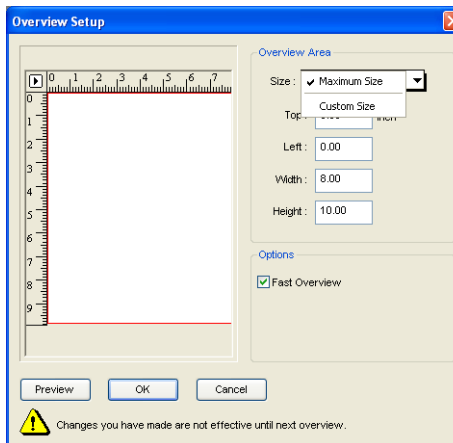

For scanning
transmissive films

As a rule of thumb, it is best to use the default maximum settings. You should change the overview area only if your subsequent overview is too large to be shown in entirety, or too small for reliable previewing. A smaller overview area will increase the overview resolution for clearer image viewing. You may also wish to change the size of your overview to improve performance. Generally, a shorter overview time results from the scanner motor travelling at a lesser distance.

Fast Overview

The Fast Overview option supports faster scanning. If Fast Overview is unchecked, the Overview scanning speed is slow, but a better overview image quality is obtained.

Overview Area


Choose Maximum Size, other fixed dimensions, or choose Custom Size, then enter the required dimensions. You may also set the Overview Area by dragging the dotted borders.

Unit

This lets you set the units for the ruler, such as inch, cm, and mm. It doesn't function for X-ray film (positive film) scanning.


Preview button

Click this button to get a scanning preview, or to do a new overview. This is helpful if you have specified custom settings or changed the dimensions.

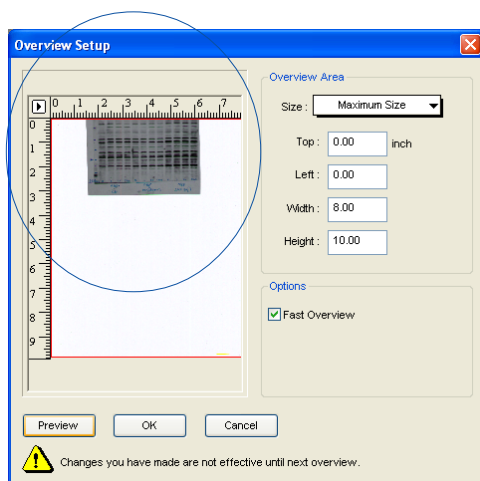

Prescan Setup

This command allows you to set the parameters for scanning a prescan image. The major difference between Overview and Prescan is that the Overview button scans the area specified in the Overview Setup command for getting a low-resolution preview image, whereas the Prescan button only scans the selected scanning frame, resulting in a more detailed preview image. When the Prescan Setup dialog box comes up, click the option you need or specify your parameters.

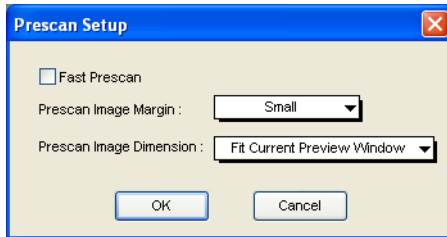

Fast Prescan

If checked, a coarser or lower-quality image is obtained but at a faster scanning speed. If unchecked, a better- quality image is obtained but at a slower scanning speed.

Prescan Image Margin


This option allows you to specify the margin around the scan job and subsequently to adjust the scan frame in the Prescan mode. Available options are: None, Small, Medium (default), and Large.

Prescan Image Dimension

This option allows you to specify the size of the prescan image. Available options are: Full screen, 75% screen, 50% screen, and Fit Preview Window. The size of the Prescan image does not necessarily fit into the specified option, as it is based only on the height/width ratio to get the maximum covered area.

Monitor Gamma Setup

The Monitor Gamma Setup command lets you compensate for the linear intensity of the monitor, allowing for consistency between the preview image and the final scanned image.

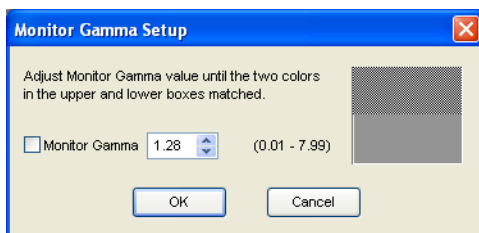



Monitor Gamma

Check this box to enable monitor gamma value setting. When the monitor gamma option is checked, click the up/down arrow buttons to make the gray level of the boxes as close as possible. Click OK to confirm.

Invert


This command creates a negative effect to an image. The Invert effect is applied to all scan jobs, not just the selected scan job.

When an image is inverted, the brightness value of each pixel is converted to its inverse value. In the case of 12-bit image, for example, a pixel in a positive image with a value of 255 is changed to 0, and a pixel with a value of 5 is changed to 250.

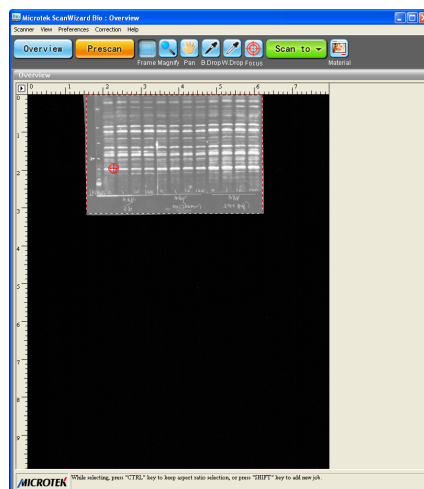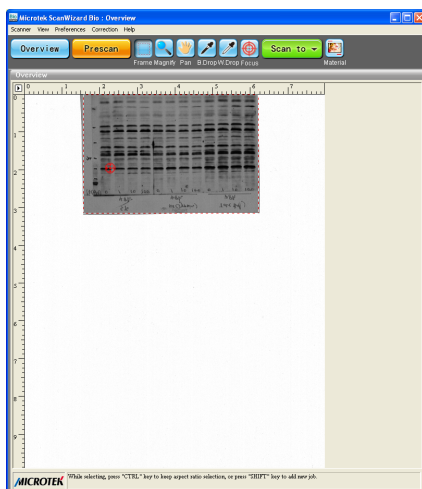

More... command

The *More...* command shows the More Preferences dialog box, where you can specify other options for ScanWizard Bio.

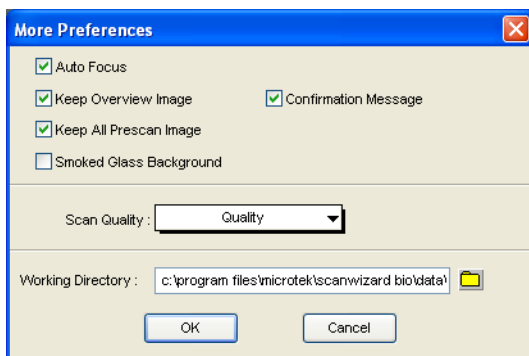

Auto Focus

If checked, the Auto Focus function tool is activated in the Preview window. If not checked, the Auto Focus function tool will be grayed out in the Preview window.

Keep Overview Image

If checked, the image that is scanned in the Overview command remains on the screen until the next image is acquisition is performed. If unchecked, the overview image is deleted when you exit ScanWizard Bio.

Keep All Prescan Images


If checked, the image that is scanned in the Prescan command remains on the screen until the next image is acquisition is performed. If unchecked, the prescan image is deleted when you exit ScanWizard Bio.

Confirmation Message

If checked, a confirmation message appears when image effects such as Rotate or Flip are applied. If unchecked, no confirmation message appears.

Smoked Glass Background

This option lets you apply a smoked glass background that makes your scan jobs stand out more clearly and allows you to focus on the scan jobs. This feature can also be used for multiple scan jobs to show their respective image modes, as well as their image editing settings.

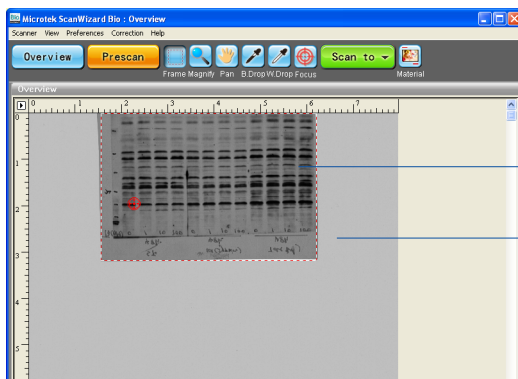

The framed part of the image (inside the marquee) stands out clearly.

Applied to the rest of the image is the smoked glass background (shaded gray area surrounding the selection or framed area).

Scan Quality

This option allows you to select the image quality by controlling the scanner hardware and the maximum image processing depth.

- Speed:** Choose this option if your primary concern during scanning is speed. Image data is delivered faster and the image data is processed in 8 bits per channel.
- Quality:** This is the default setting. Scanned data is delivered a little slower but in high quality, and the image data is processed in 8 bits per channel.
- Best Quality:** This setting is available only to higher-depth scanners (10-, 12-bit, or higher). Scanned data is delivered a little slower but in high quality, and image data is processed in maximum bits per channel (i.e., 10-, 12-bit, or higher), and then converted to the desired output depth. This special operation results in the best image quality possible.

Working Directory

This lets you specify a place to store temporary working files (e.g., scan job files) during a scanning session. If the directory you specify is not found or does not exist, a warning message appears, and ScanWizard Bio will create one automatically for you.

If the computer is shared by several users, each user may specify a particular working directory to use.

The working directory is the folder where ScanWizard Bio creates temporary files, with the temporary files deleted at the end of an operation. You should change to a different folder only if the working directory is located in a disk volume that is too small for scanning operations. To specify a new working directory, click the yellow folder beside this option, and assign a new directory to use.


Auto Background Correction (for Reflective mode only)

This option enables you to bring out and improve readability of text in a document that includes other elements such as pictures or graphs.

The Correction Menu


The Correction Menu lets you use the Advanced Image Correction (AIC) features of ScanWizard Bio. The commands in the Correction menu correspond to the AIC buttons in the Settings window.

For more information, see the section of the manual on *Advanced Image Correction*



The Help Menu

The Help menu lets you access on-line help for ScanWizard Bio, and gives you information on the ScanWizard Bio scanning software.



About

This command displays the ScanWizard Bio splash screen and shows the program's version number.




The Settings Window

The Settings window contains the parameters for outputting your scanned image for the current scan job and includes the advanced image correction tools of the program.

Elements of the Settings window

Clicking the Window Expansion button to expand the Settings window.

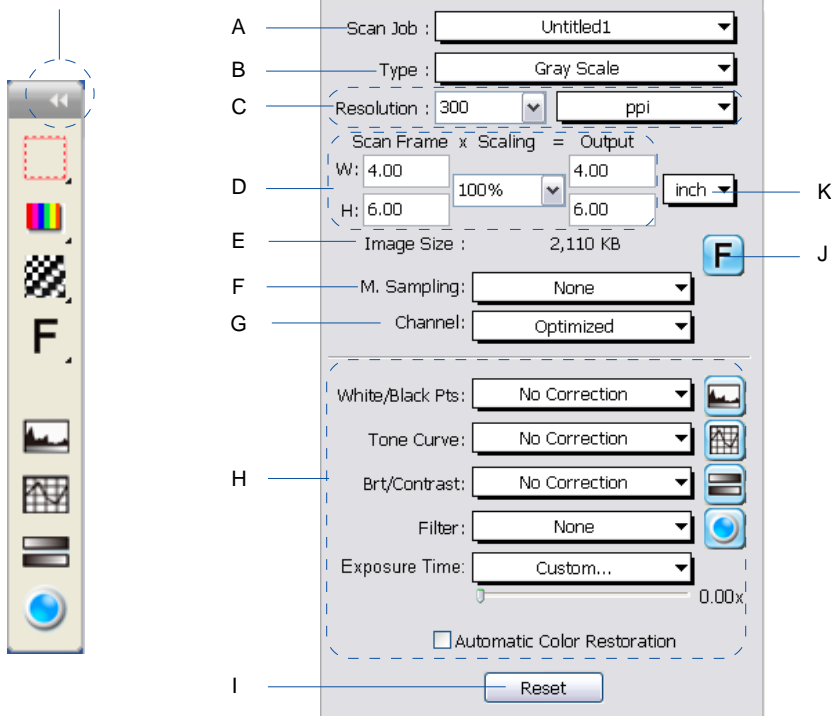

- A. Scan Job: This shows the current scan job as indicated by the Scan Job Queue window and by the selected image in the Preview window.
- B. Type: This shows the image type of the current scan job.
- C. Resolution settings: This area includes the following: the Resolution box for specifying your output resolution; the Resolution list box (with the arrow button) that provides predefined resolution values for easier selection of the resolution setting; and the Resolution unit, which lets you choose from ppi and several lpi options.
- D. Scan Frame options: This area includes the Scan Frame settings which represent the dimensions of the image that you wish to scan; the Scaling factor for creating larger or smaller images from the original source image; and the Output settings, which represent the dimensions of the image when it is output.
- E. Image size: This shows the size of the file when the image is scanned.
- F. M. Sampling (Multiple Sampling): This lets you reduce the random noise of the scanned image.
- G. Channel: This lets you to split RGB color image into a single color band.
- H. Advanced Image Correction (AIC): The Advanced Image Correction (AIC) tools let you adjust and enhance the image, and image corrections are displayed in real time. The AIC tools available for use will vary, depending on the scan material chosen in the Preview window.
- I. Reset button: This button lets specify which settings in the Advanced Image Correction (AIC) controls to be restored to their default values.
- J. Transform: This lets you flip the image horizontally or rotate the image in increments of 90 degrees. This appears only when you are prompted to perform the film scan without film holder.
- K. Unit of measurement: This lets you chose your desired unit of measurement, which will then be reflected in the rulers along side the Preview window. Choose from inch, cm, mm, point, pica, or pixel.


Scan Job

The Scan Job box shows the currently selected scan job, which is also shown in the Scan Job Queue window and the Preview window.

There is always at least one scan job in existence (by default). If you have multiple scan jobs, not only are these reflected as multiple entries in the Scan Job Queue window and as multiple images in the Preview window, they will also be shown as multiple entries in the Scan Job box of the Settings window.

To select from multiple scan jobs, choose the scan job you wish in the Scan Job box; this will automatically select the corresponding scan job in the Preview and Scan Job Queue windows as well. Conversely, selecting a scan job in either the Preview or Scan Job Queue window will automatically show that selection in the Job box.

This means that a quick look at the Scan Job box, the Preview Window, or the Scan Job Queue window can show you which is your currently selected scan job.

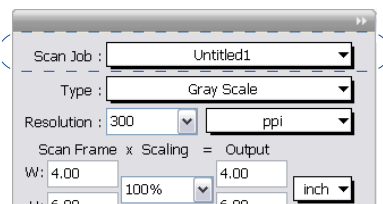

Correspondence between the Scan Job box in the Settings window and the current scan job in the Preview and Scan Job Queue windows



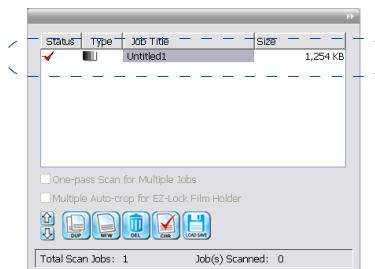


Image Type

The Type menu determines what your resulting scan will be. It does not refer to the original image type. ScanWizard Bio allows a direct scanning in either of 1D-Gray (16-bit), 2D-RGB (48-bit), Gray Scale (8-bit), or RGB Colors (24-bit) color spaces.

The default image type depends upon the scanner you are using, and the choices available to you in the Type box will also depend on your scanner.

To choose your image type, click the arrow button next to the Type box, and choose your setting from the list box.

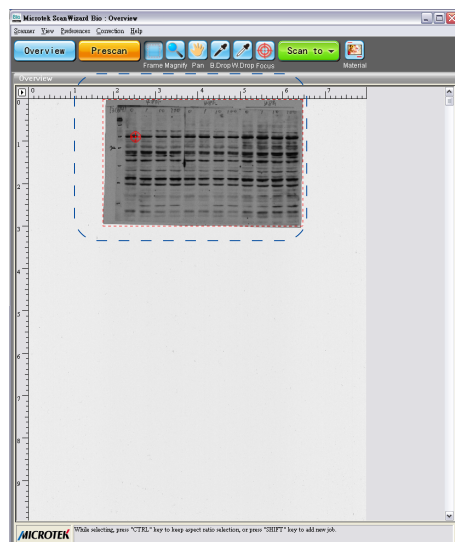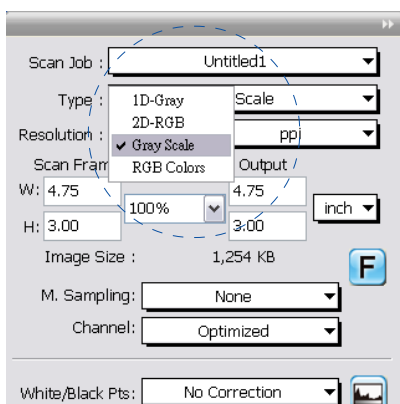

Resolution Settings

Resolution is the sampling of image pixels per measurement unit or the amount of pixel information stored in an image. Together, the image resolution and dimensions determine the file size of the image, which is measured in kilobytes (KB) or megabytes (MB).

The resolution of an image is important in determining the quality of the output image. Resolution is also directly related to file size, and the higher the resolution, the larger the resulting file size will be.

When dealing with resolution, remember to distinguish between optical resolution and interpolated resolution.


Optical resolution is the “real” resolution as measured by the scanner’s optics. Interpolated resolution is software-enhanced resolution and can be useful for enlarging very small images or for printing line art to obtain superior results.

Resolution List Box

This provides predefined resolution values for easier selection of the resolution setting.

The default resolution depends upon the scanner you are using, and the choices available to you in the resolution list box will also depend on your scanner. After you select your resolution value, this value is then recorded for subsequent use, until a new value is selected and takes over.

To choose your resolution, click the arrow button next to the Resolution box, and choose your setting from the list box.

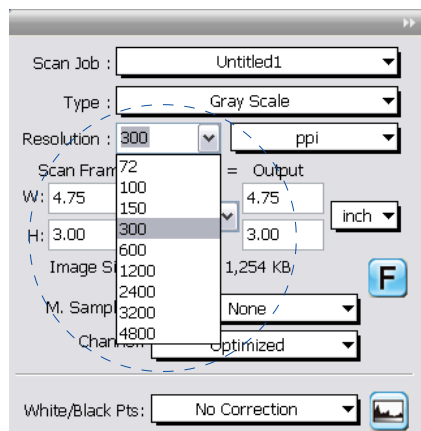


Resolution Unit

The unit of measurement for resolution is in *ppi* (pixels per inch) or *lpi* (lines per inch). Take note that *lpi* settings are dimmed if the ruler unit is in pixels.

To choose your resolution unit, click the arrow button next to the box, and choose your setting from the list box.


- Choose *ppi* if your scanned images are intended for on-screen display. In this case, you need not go higher than the target resolution of your monitor. A higher resolution value will simply increase the file size of your image without any perceptive improvement in image quality.
- Choose *lpi* if your scanned images are to be printed. If you choose 1x, for instance, your scanned image will be printed at 133 lines per inch, resulting in a 133-dpi image. At 1.5x, the image will be printed at 199.5 dpi; and at 2x, the image will be printed at 266 dpi. The Custom option allows you to set an lpi value of your own specification.

In choosing an appropriate lpi value, keep in mind that if the resolution is too low, the image becomes pixelized, resulting in a deterioration of image quality. (Pixelization is the process in which the Postscript language uses a single pixel's color values to create more than one halftone dot.) Conversely, if the resolution is too high, the file size becomes unwieldy, and your file ends up containing more information than the printer needs, slowing down the file transfer and the printing process.

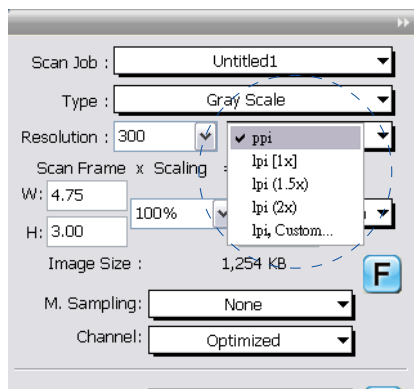

Scan Frame and Related Settings

These settings allow you to adjust the various factors that affect your image, including the width and height of your image when it is first scanned (Scan Frame settings), the Scaling factor (how big or how small the resulting scanned image will be), and the dimensions of the image when it is output (Output settings).

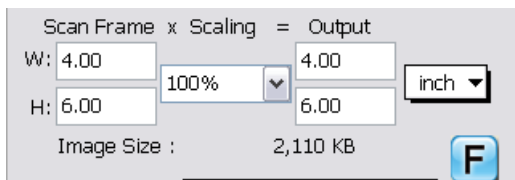

Scan Frame Settings

The Scan Frame settings (width and height) represent the area on the scan bed that you wish to scan.


To specify your settings, enter the dimensions manually in the width and height edit boxes; or use the Scan Frame tool to define or resize your scan frame. Changes made in the Preview window are automatically displayed in the Scan Frame setting edit boxes.

Scaling

Scaling lets you create larger or smaller images from the original source image. Take note of the following:

- Keep the scaling at 100% if you are outputting at the same size (e.g., a 14" x 17" original to be output at the same size).
- Reduce the scaling if you are outputting your image at a smaller size (e.g., a 9" x 7" original to be output to 4.5" x 3.5"). Increase the scaling if outputting at a larger size.

To choose the scaling percentage, click the arrow button next to the Scaling box, and choose your setting from the list box.

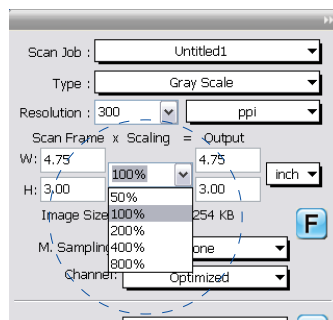

Output Settings

The Output settings (width and height) represent the dimensions of the image when it is output (to either monitor or printer). If the size of the image to be output is different from the size of the original image, adjust the scaling percentage, or manually increase/decrease the output values accordingly.

Image Size


The Image Size field indicates how big the file will be when you accept the dimensions shown in the edit boxes, together with the resolution setting that you have selected. Size is calculated automatically. The resulting file size depends on the image type; resolution; and dimensions of the image.

Unit of Measurement

The unit of measurement lets you select the desired unit (inch, cm, mm, point, pixel, pica) for your image dimensions.

To choose the ruler unit, click the arrow button next to the box, and choose your setting from the list box.

Important: Make sure you select the correct unit of measurement before entering any of the values for width or height in the Scan Frame Settings or Output Settings.

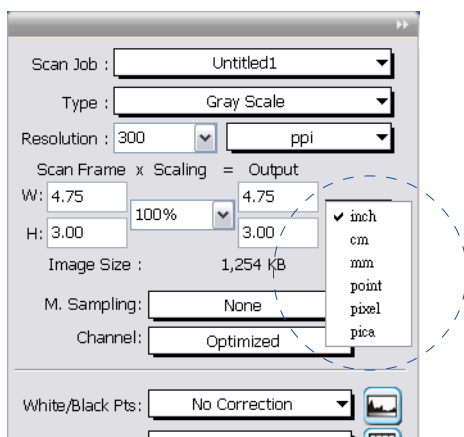


Multiple Sampling

The Multiple Sampling function is a process in which the scanner samples each line in the image a number of times, then obtains an average to reduce random noise. Enabling multiple sampling will slow down scanning, as the process requires extra time to yield higher-quality images.



To use the Multiple Sampling function,

1. In the Preview window, click the “Overview” button to preview the image.
2. Select the image area in the preview image where multiple sampling will be applied.
3. In the Settings window, click the “M. Sampling” drop-down menu, and choose an option.
4. Click the “Scan” button to start scanning. Multiple sampling is applied, producing a higher-quality image.

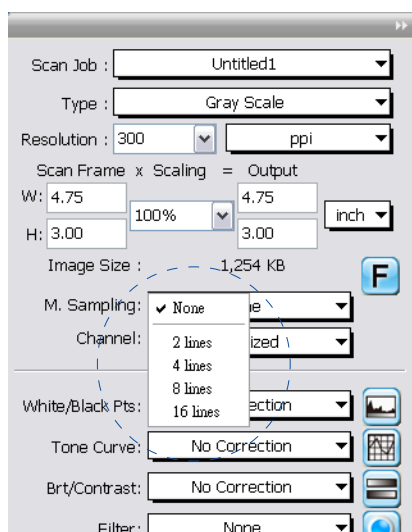


Channel


The Channel function allows you to split the RGB color image into a single color band. Use the drop-down menu to select which color band to view. This function can be activated only when the Scan Material is set as Transmissive and the Scan Type is set as 1-D Gray or Gray Scale.

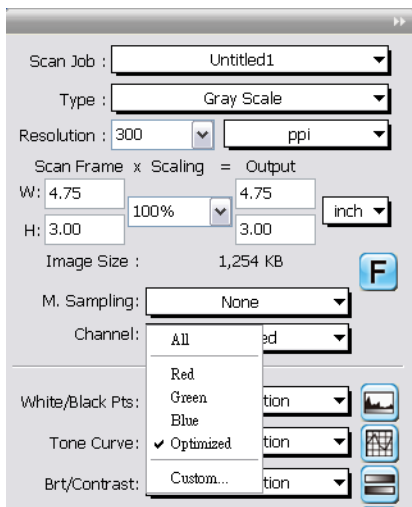

The selected "All" channels




The selected "Red" channel



The selected "Green" channel




The selected "Blue" channel



The selected "Optimized" channel (calculated by the program automatically)


Custom

The Custom option of the Channel function lets you control and adjust the portions of red, green or blue color band. When you select the option, a window appears on the screen that you can adjust the percentage for each color channel there. When done, click the OK button to carry out the action.

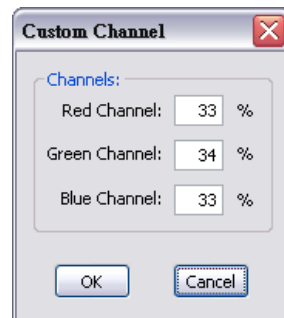


Transform

The Transform function allows you to rotate and/or flip the image in increments of 90 degrees. When you click the Transform button, a window appears on the screen to remind you that the effects of the Transform function will only be applied to the scanned image after you click the Scan button; the Transform effect is not applied to the Overview image.

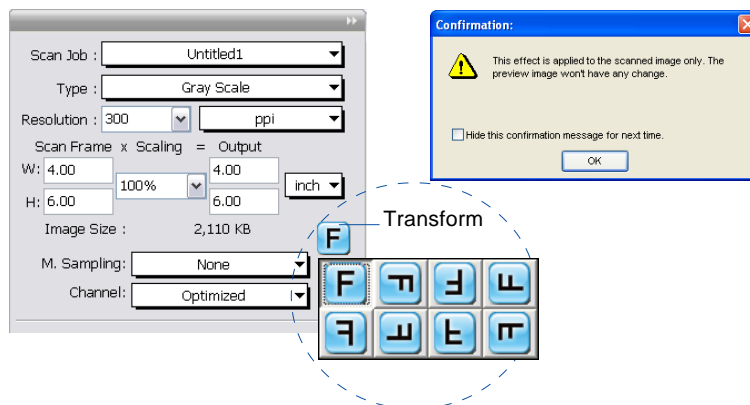

The Reset button


The Reset button in the Settings window brings up a dialog box where you can specify the AIC settings to be reset to their default values. To reset any or a combination of settings, check the boxes next to the targeted settings.

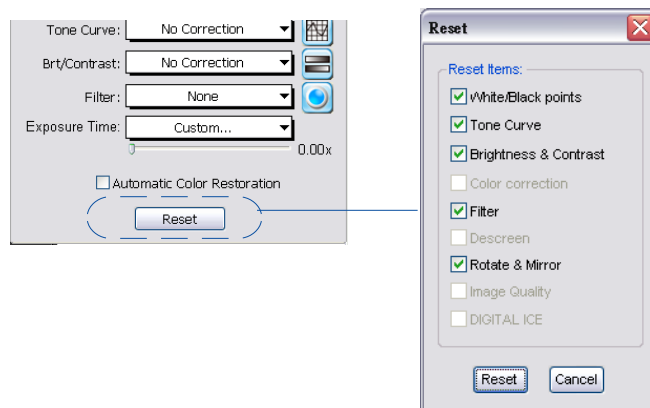


Advanced Image Correction Tools

The Advanced Image Correction (AIC) tools form an integral part of ScanWizard Bio. With the AIC tools, you can adjust or enhance images right from within ScanWizard Bio and preview the changes to your image even before you scan.

The various AIC tools available for use will be shown depending on the Scan Material chosen in the Preview window.

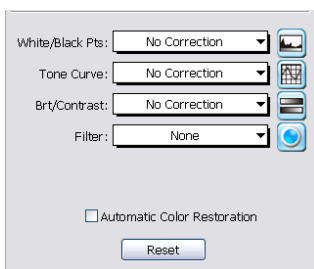

For Reflective mode only

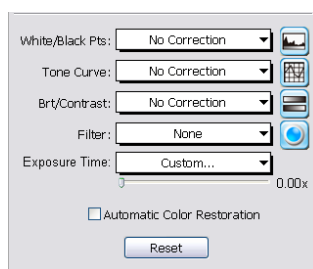



For Transmissive mode only

The following topics are covered:


- How to access the AIC tools
- Elements of the AIC dialog box
- The Action buttons
- Using Custom Settings
- Discussion of the individual AIC tools

Accessing the AIC Tools

1. To access an AIC tool, click a particular tool in the Settings window or choose its counterpart in the Correction menu in the Preview window.
2. After clicking a tool, the AIC dialog box appears. The elements of the AIC dialog box are explained in the next section.

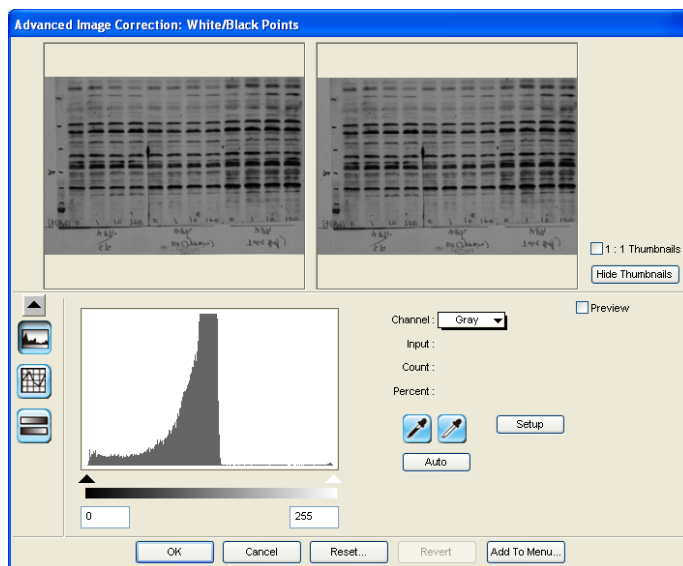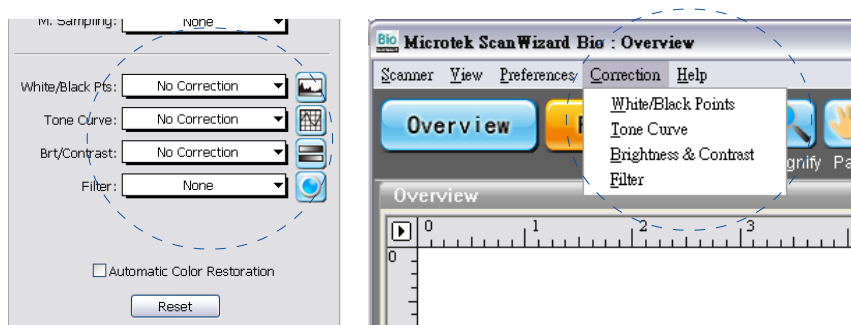

Elements of the AIC Dialog Box

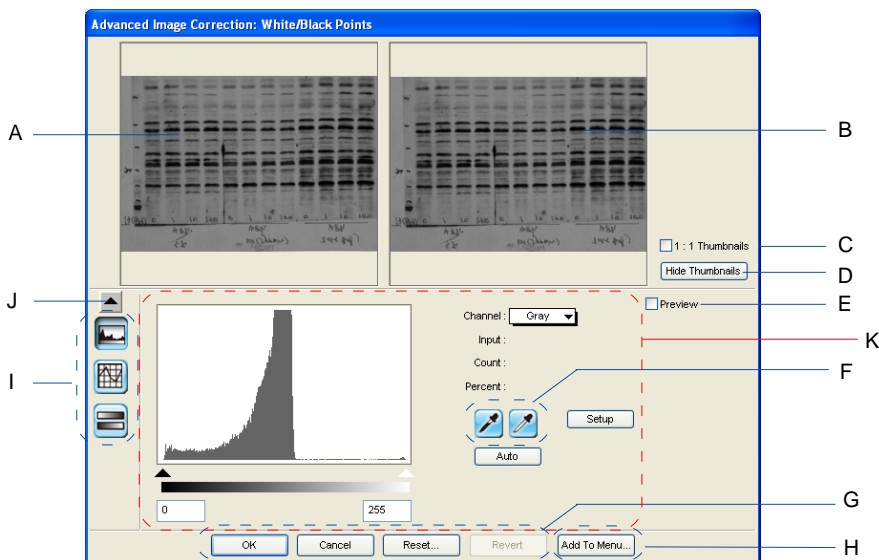

A. Left thumbnail

This shows the image *before* enhancements are applied.

B. Right thumbnail

This shows the image *after* enhancements are applied.

C. 1:1 Thumbnails

If checked, the size of the thumbnail is about the same as the image shown in the Preview window. If unchecked, the image size appears fit into the shown dialog box.

D. Hide Thumbnails

If checked, the “before” and “after” thumbnails becomes hidden. The screen collapses to show only the lower portion of the dialog box. To restore the screen, click the “up” arrow at the left side of the dialog box.

E. Preview option

If checked, changes are applied immediately to the Preview window image. If unchecked, changes are seen only after you close the AIC dialog box.

F. Function icons

These icons (e.g., eyedropper, lens, etc.) perform functions specific to the AIC tool being used. Function icons are explained in more detail under their corresponding AIC tool.

G. Action buttons

These carry out a specific action. See the next section for more details.

H. Add To Menu button

This button allows you to save a custom setting for an AIC tool. You may retrieve this custom setting afterwards from the Setting windows.

I. AIC tools

These tools adjust or enhance your images. Click any tool in this area, and see how the core of the AIC screen (#K) changes to reflect the properties of that tool.

J. Arrow button:

This allows you hide/show the thumbnails.

K. Core of the AIC screen

This is the heart of the AIC screen, and the content here changes to reflect your selected AIC tool.

The Action Buttons

The Action buttons in the AIC dialog box let you accept, cancel, or control the application of AIC settings.

OK button

This button applies to the current scan job whatever image corrections you have performed, and then closes the AIC dialog box.


Cancel button

This button cancels out all image correction changes you have made to the current scan job, and then closes the AIC dialog box. The settings remained unchanged

Reset button

This button brings up the Reset dialog box, where you can specify which settings are to be restored to their default values, then click Reset or Cancel.

If Reset is selected, the settings are restored to their default values; if Cancel is selected, the operation has no effect.

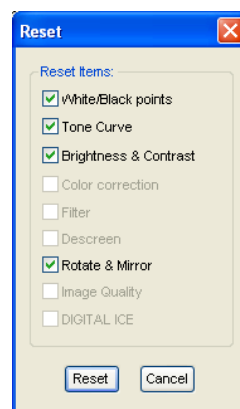


Revert button

This button to cancel out the changes that were made with the current image correction tool. This means that if you used several AIC tools, Revert cancels the effect of only the last used (or current) tool, and preserves the effects of the other preceding tools.

Custom Settings

When you click on each AIC setting in the Settings window, a drop-down menu will show options for adding, removing, or loading custom settings. These custom settings are settings that you define yourself for your scan jobs.

For instance, if you wish to change the shadow to an image and then save that shadow setting for future scan jobs, you can add the shadow setting as a custom setting. The next time you wish to retrieve that particular shadow setting, simply go to the White/Black Point AIC drop-down menu, and choose that setting.

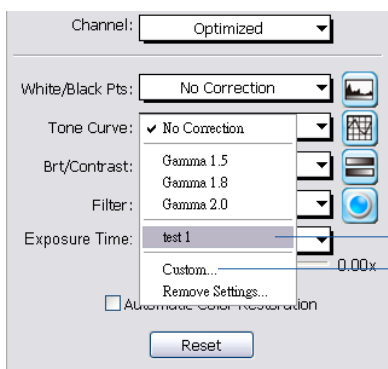


A user-defined setting that has been added and can now be retrieved

Lets you add or remove from the menu settings you have previously defined


Adding Custom Settings

To add a custom setting for an AIC tool, click the *Custom...* in that tool's pop-up menu, or click the *Add To Menu ...* button in that tool's dialog box. When a dialog box comes up, enter the name of the new custom setting to be added. For instance, the added setting can be called “test 1” as shown below.

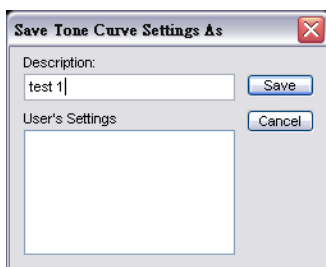


Removing Custom Settings

To remove a custom setting for an AIC tool, click the *Remove Settings...* in that tool's pop-up menu. When a dialog box comes up, select the particular setting to be removed, then click *Remove* and *Done* in the dialog box.

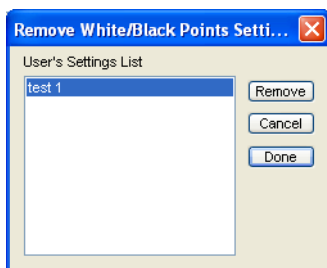

Loading/Retrieving Custom Settings

To load or retrieve a custom setting that you have previously defined for an AIC tool, go to that AIC tool's pop-up menu, and choose the setting you wish to be loaded.

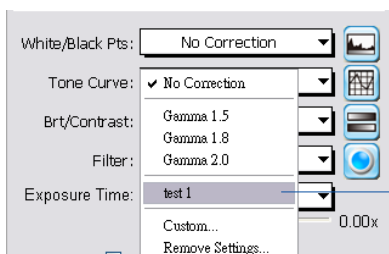


Custom setting to be retrieved or loaded

White/Black Points

The White/Black Points tool is used to change the shadow and highlight points of an image.

By using this tool, you can manipulate an image to either bring out the highlights in a very dark image, or bring out more of the shadows in a very light image. The White/Black Points tool can also be used to neutralize the color cast in the highlight and shadow regions.

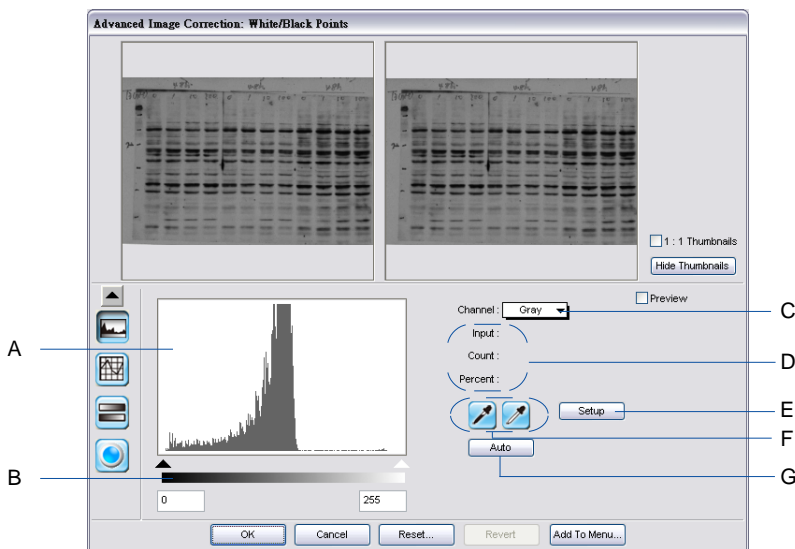

A. Histogram

The histogram is a graphic representation of how all the pixels in an image are distributed across brightness and darkness levels. The darkest pixels are at the left; the lightest pixels are at the right.

A histogram skewed heavily to the left indicates that the image has many more dark pixels than light. Conversely, a histogram skewed heavily to the right will indicate a light image as it has more light pixels than dark. The height of the histogram indicates the number of pixels at that point in the histogram.

B. Sliders

The sliders are used to adjust the Black and White points of the image. The values of the black and white points are reflected in the edit boxes below.

C. Channel

The channel allows you to control the shadow and highlight settings for Gray channel.

D. Input, Count, Percent

These figures provide information about the histogram. The figures will appear only when the cursor is on the histogram or if a slider is being moved.

- The Input value indicates the color value of the data displayed in the histogram.
- The Count value indicates the number of pixels at the Input value. If Input value is 2 and Count value is 1300, then there are 1300 pixels in the image at the Input value of 2.
- The Percent value is the percentage of all pixels in the image where color value is less than or equal to the input value. For example, if Percent is 15% and Input value is 2, it means that 15% of all pixels in the image have a value of 2 or less.

E. The Setup button

This button provides you with advanced controls for setting the clipping points for your white/black points, as well as determining the output levels for the white/black points on your printer.

Click to bring up the White/Black points setup dialog box. For more details, see the section titled *White/Black Points Setup* (under the Preferences menu in the Preview window).

F. Pickers

The Pickers can be used instead of the sliders to set the Black and White points, based on color values in the preview image. The Picker on the left sets the Black point; the Picker on the right sets the White point.

- To set the White point: Click the Picker on the right, then click on the preview image to define the reference point.
- To set the Black point: Click the Picker on the left, then click on the preview image to define the reference point.

G. Auto button

The Auto button automatically judges the darkest and whitest points and clips excessive black or white points. The clipping percentage of the white/black points is accessible by clicking the Setup button.

Using the White/Black Point tool:

1. Choose the Channel in which the histogram will be modified.
2. Move the black and white sliders to new points on the histogram.
 - Moving the black slider to the right will yield more contrast in the highlight areas of the image, so that more detail emerges in the highlight areas.
 - Moving the white slider to the left will yield more contrast in the shadow areas of the image, so that more detail emerges in the shadow areas.


Another alternative is to simply click the Auto button, so that the shadow and highlight for the image is determined automatically.

3. When the changes are done, click OK.

For more details on the effects of the other action buttons, see the section “The Action Buttons”.

Tone Curve

The Tone Curve tool lets you adjust the tonal range of an image. However, instead of making adjustments using just three variables (highlights, shadows, and midtones), you can adjust any point along the 0-to-255 scale (for 8-bit images; 0-to 4096 scale for 12-bit images).


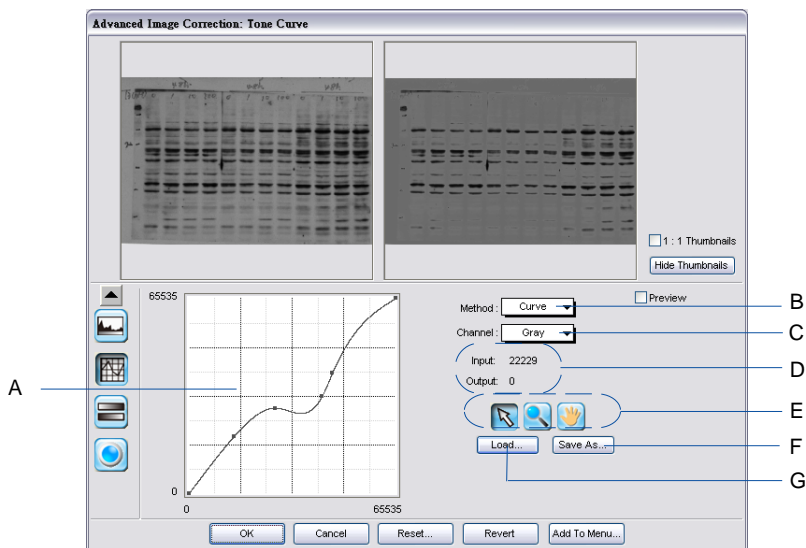


How to Read the Curve



The Curve shows the relationship of the brightness changes across the middle pixels between the resulting image and the original. When you open the Curves dialog box, the line on the graph is diagonal because the Input and Output values are the same.

When the curve is moved up or down, the relationship between input value and output value changes accordingly.

- In areas where the curve is moved down, pixels in that portion of the image are darkened.



- In areas where the curve is moved up, pixels in that portion of the image are lightened.




Contrast in an image can be seen by the angle of the line. The steeper the slope, the higher the contrast. The closer the line is to horizontal, the lower the contrast.

A. Curve

The Curve is a graphic representation of the tone curve showing scanner input from dark on the left to light on the right.

B. Method

The Method sets the kind of curve you wish to have. Select from Line, Curve, or Gamma.

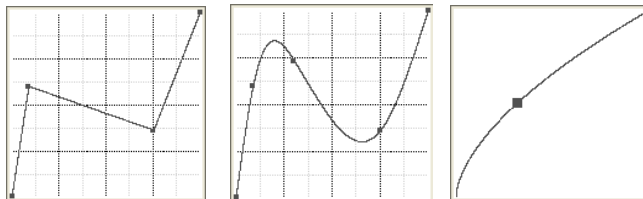

C. Channel

The Channel allows you to choose the gray channel only in which the gamma will be affected.

D. Input, Output, Zoom:

- Input shows the horizontal value of wherever the cursor is inside the curve, reflecting the scanner's full depth.
- Output shows the vertical value of wherever the cursor is inside the curve, reflecting the scanner's full depth.
- Zoom indicates the magnification level of the curve box. At 100% zoom, the curve is seen in its entirety. Using the zoom frame tool to magnify the curve will zoom in or enlarge your view of the curve, resulting in a higher zoom percentage.

E. The Curve Tools

The Curve Tools let you modify the curve. The tools are the curve pointer, the curve zoom frame, and the curve pane.



Use the Curve Pointer tool to define points in the curve that will be modified. When you click on any point in the curve, a black handle appears to mark your position. To remove the handle, drag it off the graph.



Use the Curve Zoom Frame tool to zoom in and out on a particular point in the curve. Once the area is zoomed in, you can then use the Curve Pointer tool to define new points for better precision. This is particularly useful for working with 12-bit images, where more detail can be seen in such images. The zoom level can be seen in the Zoom field. To zoom out, click Shift.



Use the Curve Pane tool to scroll through the curve if the curve has been zoomed in. This curve tool can be used only if the curve has been zoomed in with the Curve Zoom Frame button (above). Otherwise, the Curve Pane tool will be dimmed.

F. The Save As button

The Save button lets you save a tone curve together with its settings so that the curve can be used in the future if necessary.

G. The Load button

The Load button lets you load a previously saved tone curve for use with another image. Photoshop-saved curves can also be loaded.

Using the Tone Curve tool:


1. Choose the Channel in which the curve will be modified.
2. Choose the Method in which the curve will be modified. Select from Line, Curve, or Gamma.
3. Click the Curve Pointer tool, then click on the curve to define the points where the curve will be modified. You can then either raise or lower the curve at that point and see changes to the image accordingly.
4. When the changes are done, click OK.

For more details on the effects of the other action buttons, see the section “The Action Buttons”.

5. To save a curve, click the Save As button. To load a previously saved curve, click the Load button and specify the curve setting to be loaded.

Filter

The Filter tool is used to apply special effects to an image. Several filters are provided in ScanWizard Bio, including None, Blur/Blur More, Edge Enhancement, Emboss, Sharpen/Sharpen More, Unsharp Masking and Sharpen Low/Medium/High.

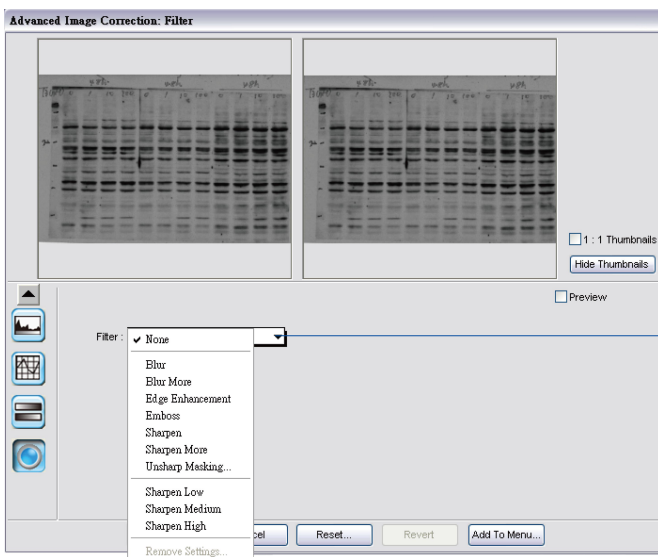

Click the drop-down menu to select the filter you want to apply to your image

- Blur/Blur More: The Blur filters decrease the contrast between adjacent pixels, making the image appear hazy and out of focus.

Both Blur and Blur More filters make images look softer, with the Blur More filter having a stronger blurring effect than the Blur filter.

- Edge Enhancement: The Edge Enhancement filter gives greater contrast to edges. The filter can do this because edges are areas in an image where gray or color levels change abruptly. It is best to use this tool for improving geometrical contoured shapes.
- Emboss: The Emboss filter uses a technique in which each pixel of an image is replace either by a highlight or a shadow, depending on light/dark boundaries on the original image. Low contrast areas are replaced by a gray background. The filtered image will represent the rate of color change at each location of the original image.


- Sharpen/Sharpen More: The Sharpen filters increase the contrast of adjacent pixels, making images appear sharper and more focused.

Both Sharpen and Sharpen More filters improve clarity, with the Sharpen More filter having a stronger sharpening effect than the Sharpen filter.

- Unsharp Masking: The Unsharp Masking filter is used to adjust the contrast of edge detail, creating the illusion of more image sharpness. This filter can be useful for refocusing an image that has become blurry from interpolation or scanning, and it is an essential tool for doing CMYK color separation. In general, Unsharp Masking is needed to render sharp color reproductions, especially when you wish to make a large color reproduction from a small original.

To adjust the contrast of edges, follow the steps below:

1. Choose Unsharp Masking to open its dialog box from the Sharpen options menu.
2. Enter a value in the Strength box to specify the degree of the filter's effect. The higher the value, the stronger the effect of the filter.

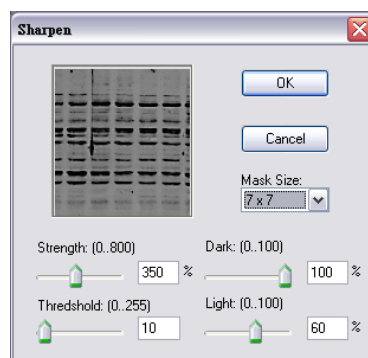


3. Select a mask size in the Mask Size box. This parameter determines the depth of pixels that will be affected at the edge. Available selections are 3x3, 5x5, 7x7, 9x9, 11x11, and 13x13. For small, low-resolution image files, 3x3 is sufficient. For high resolution, or large-scale image files, use 7x7.
4. Enter a value in the Threshold box. This option allows you to specify a tolerance range to prevent overall sharpening that might generate noise or cause other unexpected results. The Threshold defines the required contrast between adjacent pixels in an image before sharpening is applied to an edge. A lower value produces a clearer effect.
5. Click OK to apply the settings.

- Sharpen Low/Medium/High: The Sharpen filters increase the contrast of adjacent pixels, making images appear sharper and more focused.

Three of these Sharpen filters improve clarity, with the Sharpen High filter having a strongest sharpening effect among all.

Brightness and Contrast

The Brightness & Contrast tool lets you control the brightness and contrast levels of the entire image. Increasing the brightness makes all tones in the image lighter. Contrast, on the other hand, is the range between the darkest and lightest shades in the image, and increasing the contrast makes greater separation between the darkest and lightest areas of the image.

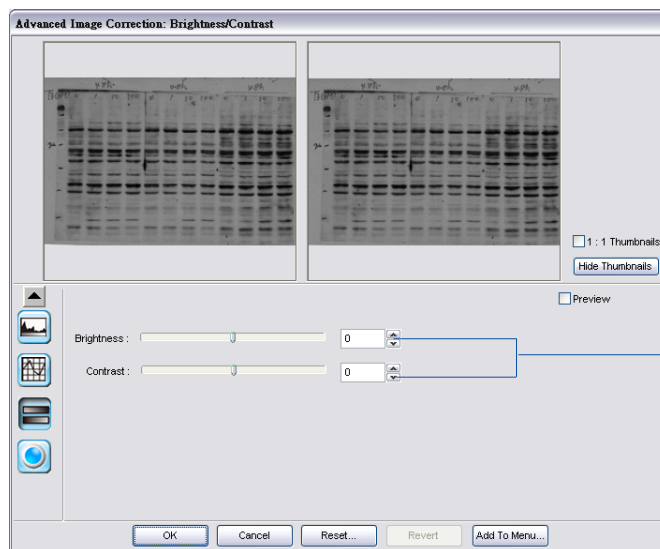


Drag the sliders or enter values to change Brightness and Contrast

- **Brightness:** The Brightness control lets you change the brightness setting. Too much brightness can make an image look washed out, while too little brightness will make the image look dark.
- **Contrast:** The Contrast control lets you change the contrast setting. Too much contrast will make an image look like a photocopy of a picture, with little or no gray shades left. Too little contrast will make the colors in the image look dull and flat.

Exposure Time (for Transmissive mode only)

The Exposure Time tool allows you to perform the exposure correction for the current scan job. This function tries to average the intensity of the image and to compensate for a very dark image, making the dark areas of the image much brighter.

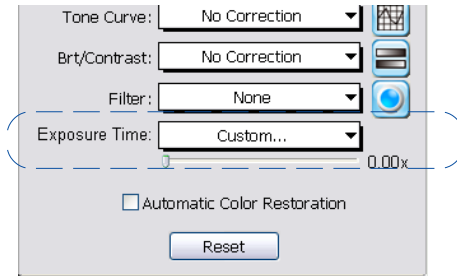

Custom...

This allows you specify a custom setting for the Exposure Time to your image.

Using the Exposure Time,


1. In the Settings window, click the arrow button next to the Exposure Time box, and choose “Custom...” to enable its slide bar under it.
2. Point your mouse to the slider bar, then adjust slider bar to increase/decrease the value of a user setting.

The value of the exposure is reflected by the slider bar after you made adjustment. A high exposure value will extend scanning processing time, for it requires extra time to produce a better visible image.

Note: The Exposure Time function is available only in the Settings window when the connected scanner is supported by this function (e.g., Bio-5000).

Automatic Color Restoration

The Automatic Color Restoration feature allows the scanner restores faded colors in photos or films, bringing hues back to their original luster and brilliance for more vibrant images. With one-click, automatic color recovery process is simple and straightforward, involving no learning curve or hassle.

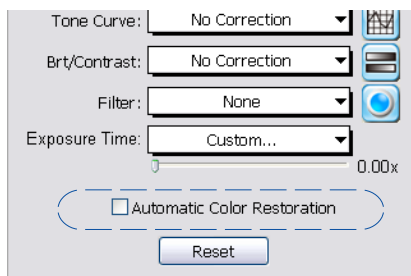


To use the Automatic Color Restoration function:

1. In the Preview window of the Advanced Control Panel, marquee the faded image area to be restored.
2. In the Settings window, check the “Automatic Color Restoration” option.
3. Click the “Scan To” button to perform scanning. Automatic Color Restoration is applied, and faded colors in the photo are restored.

The Information Window

The Information window displays color information as you move the cursor over the preview image in the Preview window (or the thumbnail in the Advanced Image Correction dialog box if it is open).

You can choose to show or hide the Information window in ScanWizard Bio. To do this, click the *Show/Hide Info window* toggle command under the View menu in the Preview window.

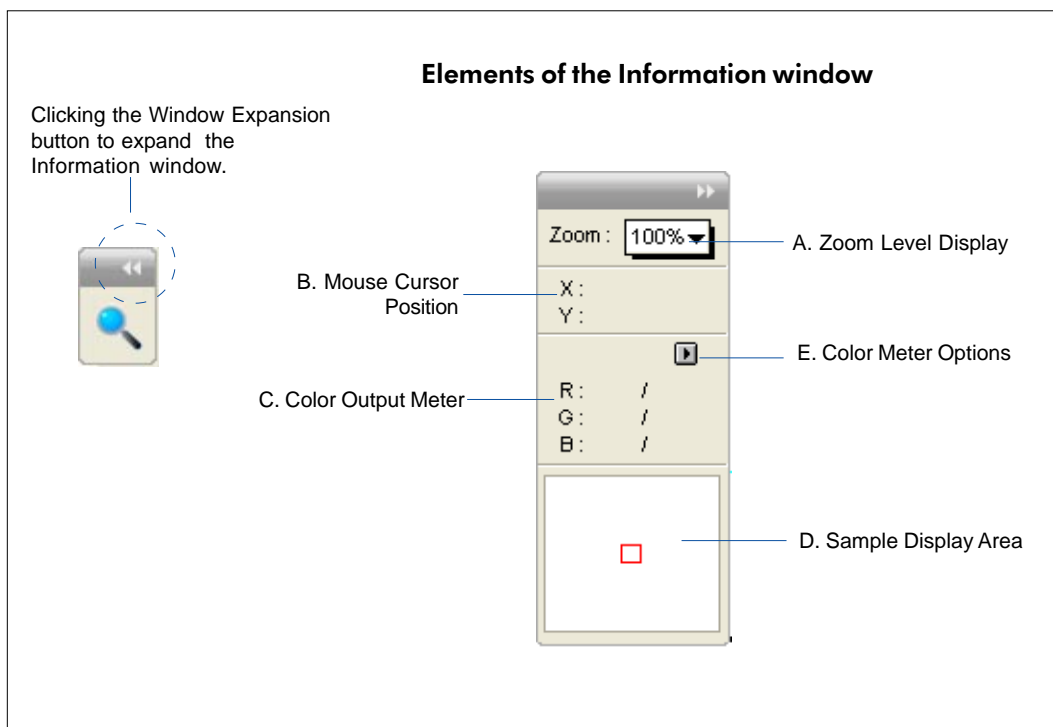


A. Zoom Level Display

The Zoom Level Display magnifies your view of an image, much like the Zoom (Magnify Glass) tool in the Preview window.

The magnification factor in Zoom Level Display is by a factor of 2. Thus, the magnification levels increase from 100% to 200%, to 400%, to 800%.

To use the Zoom Level Display, click the Zoom box to choose a zoom or magnification level you wish to use from the drop-down menu that appears.



B. Mouse Cursor Position

The Mouse Cursor Position (Pixel Position) shows you the cursor position on the x (horizontal) and y (vertical) coordinates of the axis. This feature is useful for operations that require very precise measurements and alignment.

C. Color Output Meter

The Color Output Meter is useful if you wish to adjust the shadow and highlight points of an image.

As you move the cursor over a point in the image, the Color Output Meter will show the appropriate K values of that point in the image. The significance of the numbers is explained below.

- There are two numbers shown in the Color Output Meter. The first number represents the raw color data taken by the scanner; the second number represents the resulting value after color correction or image enhancement is applied to the image.
- The values can be anywhere from 0 to 255, with 0 as the black point, 255 as pure white, and all other values in between corresponding to shades of varying degrees between black and white.
- The values as a whole represent color info for the sample size selected in the Color Meter Options button. For instance, if you chose 3 x 3 as your sample size and your K value reads 23, that shows your K value of 23 is the average of a 3-pixel by 3-pixel area.

Pixel-value info is useful especially if you are making color corrections based on color values. Knowing this, you can modify the shadow and highlight points of an image, then come back to the same point in the image, and verify through the Color Output Meter that the K values have indeed changed.


D. Sample Display Area

This shows a pixelized display of the area surrounding the cursor. The size of the sample area depends on the selection made in the Color Meter Options.

E. Color Meter Options

These options let you choose how color information is displayed — in numbers or percentages.

To use the Color Meter Options, click the Color Meter Options button to choose your setting from the drop-down menu that appears.

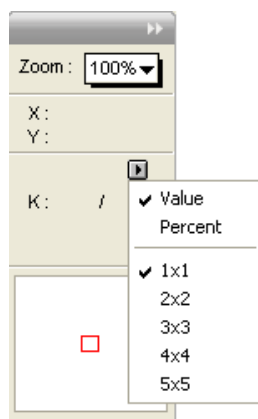

Value and Percent

- If *Value* is chosen, the numbers represent values in the 0-to-255 pixel scale regardless of the bit depth of your output image.
- If *Percent* is chosen, the numbers represent the percentage of intensity.

Color Meter Options


The Color Meter options let you choose the size of your sample display area. For instance, if you choose 5 x 5 as your sample area, this means your K value will represent color information for a 5-pixel by 5-pixel area. If you choose 1 x 1 (the default), the color information pertains to a single pixel — the pixel in the middle of the sample area.

Scan Job Queue Window

The Scan Job Queue window provides several functions for managing your scan jobs. By definition, a scan job contains the following elements: a set of scanning parameters (shown in the Settings window); a scan frame (shown in the Preview window); and one or several scan job items (shown in the Scan Job Queue window).

You can have multiple scan jobs, each having its own distinct settings; the number of scan jobs is indicated by the number of titles in the Scan Job Queue window (two in the example below). Scan jobs marked with a check are the ones designated to be scanned, and the jobs are scanned in the order that they appear in the Scan Job Queue window.

You can choose to show or hide the Scan Job Queue window in ScanWizard Bio. To do this, click the *Show/Hide Scan Job Queue window* toggle command under the View menu in the Preview window.

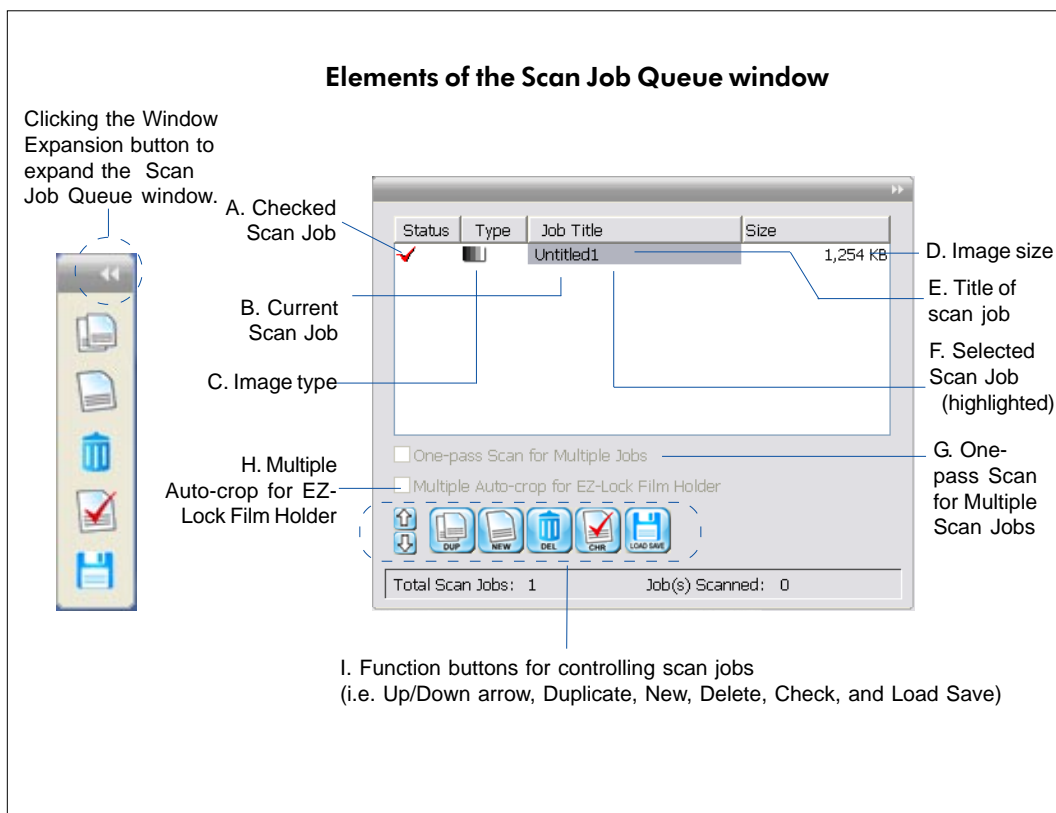

- A.. Checked scan job: Checked scan jobs are the ones that are scanned when you click the *Smart-Scan button* or *Scan to* button in the Preview window. To check a scan job, you can either click the Check icon or use the *Check* button at the bottom of the Scan Job Queue window.
- B Current scan job: This is the current scan job, indicated by a frame around the title. There may be several defined scan jobs, but only one scan job can be current. In the Preview window, the current scan job is the one with the flashing marquee.
- C. Image type display: This shows the image type of the scan job .
- D. Image size: This is the image size of the scan job.
- E Title of scan job: The title of each scan job is shown. To edit a scan job title, double-click the title of scan job and type a new name when an edit box appears.
- E Selected scan job: The selected scan job is the highlighted item. You can have multiple selected scan jobs, and clicking on a function button (such as *Check* or *Duplicate*) will implement that function on the selected scan job.
- G. One-pass Scan for Multiple Scan Jobs: This allows the scanner performs scanning in a single pass for all the selected scan jobs.
- H. Multiple Auto-crop for EZ-Lock Film Holder: This allows the scanner automatically performs an Auto-crop after scanning multiple films at one time.
- D. Function buttons for controlling scan jobs: These buttons perform a specific action on the selected scan job. The *Duplicate*, *New*, *Delete*, *Check* and *Load/Save* buttons can be used on multiple selected scan jobs.
- E. Thumbnail of prescan image: A thumbnail (Ⓢ) appears for the selected scan job after you click the *Prescan* button in the Preview window. This means a prescan image is available for that scan job. This function is available only in the Reflective mode.

One-pass Scan for Multiple Scan Jobs

This option is enabled only when the scanner model you are using supports the one-pass scan function. Otherwise, this option is disabled and grayed out.

If this option is unchecked, when you assign multiple scan jobs in the preview window, the scanner will continuously scan for several passes, depending on the number of scan jobs that are selected. For instance, assuming that there are three scan jobs selected, the scanner performs the first job, and as the scanner carriage returns to the stand-by position, the scan for the second job begins, and so forth to the third job — for a total of three passes. More scan jobs there are, the longer the scanner time will be.

If this option is checked, the scanner performs scanning in a single pass for all the selected scan jobs. The scanner's carriage moves only once and when it returns to the stand-by position, ScanWizard Bio then starts to process and finish all of the scan jobs.

To use the “One-pass Scan for Multiple Jobs”, the image original should meet the following conditions:

1. For all the scan jobs, the “resolution x scale” value in the Settings window should be the same.
2. All the scan jobs should have the same scan type.
3. If the screen filter is applied, all the scan jobs should use the same descreen lpi value.

If ScanWizard Bio has detected that your image original does not meet the above conditions, the “One-pass Scan for Multiple Jobs” option is dimmed and will not be available for selection.

Multiple Auto-crop for EZ-Lock Film Holder

This option is enabled only when the EZ-Lock film holder (or medical series film holder) is placed on the scanner glass surface, and the scan material is set as Transmissive. Otherwise, this option is disabled. Check this option to enable the scanner to auto-crop multiple scanning frames.

To perform multiple auto-crop preview of the film loaded onto the scanner, click the Smart-Scan button. When done, you will see multiple scan frames that have been automatically cropped in the preview window. Multiple job titles will appear in the Scan Job Queue window, numbered sequentially and all marked by a “Check” that indicates the jobs are ready to be scanned.

Note: After performing multiple auto-crop scanning, the previously created jobs will be removed from the Scan Job Queue window.

Function Buttons



Selecting Multiple Scan Jobs

The *Duplicate*, *Delete*, and *Check* buttons at the bottom of the Scan Job Queue window can be used for multiple job selections.

For example, you can select multiple scan jobs, and then click the *Delete* button to remove all the jobs simultaneously.

To select multiple scan jobs, press the *Ctrl* or *Shift* key and click on the jobs to be selected.

Editing Multiple Scan Jobs

ScanWizard Bio lets you edit multiple scan jobs at the same time, increasing your efficiency in using the software.

To edit multiple scan jobs, simply select all the scan jobs to be edited in the Scan Job Queue window.

To include each scan job for selection, use the *Shift* + Click combination (pressing the *Shift* key while clicking the mouse at the same time). Then perform the selected editing function.

For instance, you can go to the Settings window and choose an image type that will apply to all the scan jobs. Another example is to apply a common resolution setting to all the scan jobs. Simultaneous editing simplifies the scanning process for you.



Adding a New Scan Job

The New button lets you create a new scan job; the new scan job will have default settings. This feature allows you to create as many scan jobs as you wish, and each scan job can then have its own settings.

1. Click the *New* button.
2. When a title of new scan job appears, accept the default name or enter a name for the new scan job. Use unique names for your scan jobs, as duplicate names are not accepted.
3. Define the scan frame in the Preview window for the new scan job.
4. In the Settings window, specify the settings for the new scan job. With the creation of a new scan job, the new scan job becomes the current scan job.



Duplicating a Scan Job

The Duplicate button lets you duplicate the settings of a scan job. This function is very helpful if you have created optimal settings for a scan job and wish to use these settings as a template for other scan jobs. This saves time, as you don't have to create the settings repeatedly for every scan job you make.

1. From the list of scan jobs available, select the scan job(s) to be duplicated.
2. Click the *Duplicate* button. The selected scan job(s) will be duplicated. The Duplicate function is very useful when scanning several images at the same settings.



Removing a Scan Job

The Delete button allows you to remove a scan job from the list of scan jobs available.

To delete a scan job, highlight the scan job to be removed, then click the *Delete* button.



Checking a Scan Job

The Check button allows you to select the scan jobs to be scanned. Checked scan jobs are the ones that are scanned when you click the *Smart-Scan button* or *Scan to* button in the Preview window. The check button is a toggle for checking/unchecking a scan job.

To check a scan job, highlight the scan job, then click the *Check* button. A check sign will appear next to the selected scan job.

To uncheck a scan job, highlight the scan job, then click the *Check* button. The scan job will be unchecked, and the scan job will not be scanned when you click on the Scan button.



The Up/Down Arrows

The Up/Down arrows allow you to change the order of the scan jobs in the Scan Job Queue window.

To move up/down the scan job, highlight the scan job, then click the Up/Down arrow to change the order of the scan job in the list.

When you start scanning, the scan jobs will be processed and scanned in the order that they appear in the Scan Job Queue window.




The Load/Save button

The Load/Save button allows you save scan jobs that can be loaded at a later time when necessary. The idea of saving and loading scan jobs has important applications, especially for scanners with different templates or “trays”. Loading/ Saving scan jobs is also useful if you consistently work in a specific format, scan the same kind of images, or if the scanner is used by several users who have their own sets of jobs.

To save a scan job as a template:

1. Click on the *Load/Save* button to open the Job Template Manager window.
2. Specify a folder for saving scan jobs by clicking the Folder icon (yellow) or use the current default folder.
3. Highlight the scan jobs you want to save at the right column of the window.
4. Click the <<Save button in the window. The selected scan jobs will be saved into the chosen folder and appeared at the left column of the window.

You may also specify different folders for respective scan job templates as you desired.

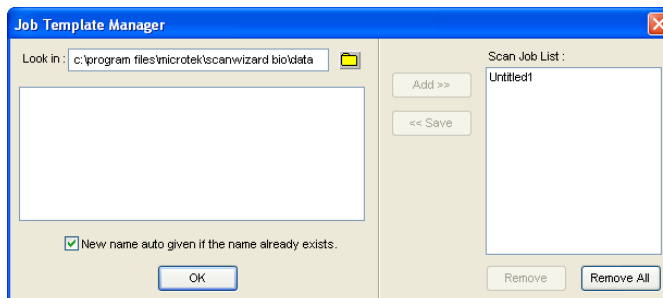

To load a scan job template:

1. Click the *Load/Save* button to open the Job Template Manager window..
2. Switch to the folder where the scan job template is stored.
3. Highlight the scan job template to be loaded at the left column of the window.

Before loading a new scan job, you may remove your existing scan jobs from the right column

4. Click the *Add>>* button in the window to load the scan jobs from a chosen folder into the Scan Job Queue window.

To remove a scan job template:

1. Click the *Load/Save* button to open the Job Template Manager window.
2. Highlight the scan job to be removed at the right column of the window.
3. Click the *Remove* or *Remove all* button in the window to remove the scan job from the Scan Job Queue.

New name auto given if the name already exists

When you load or save scan jobs, you may check or uncheck the “New name auto given if the name already exists” option in the window. Suppose the scan jobs already exist, if you check this check box, the number suffix is automatically appended as a new scan job. If unchecked, the existing scan jobs are overwritten.

Appendix

Product and Technical Support

If you need to call Technical Support, please have the following information ready:

- Your scanner model. The scanner product name is indicated on the front (or top) of the scanner, not the back.
- The scanner's serial number. This can be found on the back panel of the scanner.
- Your computer name and model.
- The version number of ScanWizard Bio. This is indicated on the ScanWizard Bio scanning software.
- Your system components, or the devices on your system, such as an external hard drive, CD-ROM, etc.
- Software being used with your scanner.

Important

Aside from having the above information ready, please make sure that when calling technical support, you (or someone calling for you) are knowledgeable about the basic operations that may need to be performed on PCs. These procedures include:

- How to edit the CONFIG.SYS file
- How to edit the Windows WIN.INI file

Microtek's technical support will not walk you through these procedures. You are assumed to have knowledge of your Windows system.